

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022224\
 Data File : VW034342.D
 Acq On : 22 Feb 2024 13:12
 Operator : SY/MD
 Sample : P1498-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB7

Quant Time: Feb 23 01:16:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 23 01:14:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	82967	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	78139	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.184	152	36988	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	19684	3.063	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	61.200%	
7) Chloroethane-d5	1.535	69	20079	3.568	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	71.400%	
11) 1,1-Dichloroethene-d2	2.059	65	10987	3.546	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	71.000%	
20) 2-Butanone-d5	3.812	46	54118	50.148	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	100.300%	
24) Chloroform-d	4.252	84	52269	4.477	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	89.600%	
26) 1,2-Dichloroethane-d4	4.947	65	26870	4.924	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	98.400%	
32) Benzene-d6	4.963	84	93097	3.971	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	79.400%	
36) 1,2-Dichloropropane-d6	5.989	67	27911	4.259	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	85.200%	
41) Toluene-d8	7.246	98	85410	3.964	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	79.200%	
43) trans-1,3-Dichloroprop...	7.564	79	7451	3.011	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	60.200%	
46) 2-Hexanone-d5	8.030	63	41490	46.969	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	93.940%	
56) 1,1,2,2-Tetrachloroeth...	10.152	84	18828	4.739	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.800%	
66) 1,2-Dichlorobenzene-d4	11.561	152	31659	4.706	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	94.200%	
Target Compounds						
22) cis-1,2-Dichloroethene	3.818	96	35024	5.229	ug/L	98
34) Trichloroethene	5.844	95	4453	0.657	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022224\
Data File : VV034342.D
Acq On : 22 Feb 2024 13:12
Operator : SY/MD
Sample : P1498-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB7

Quant Time: Feb 23 01:16:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 23 01:14:23 2024
Response via : Initial Calibration




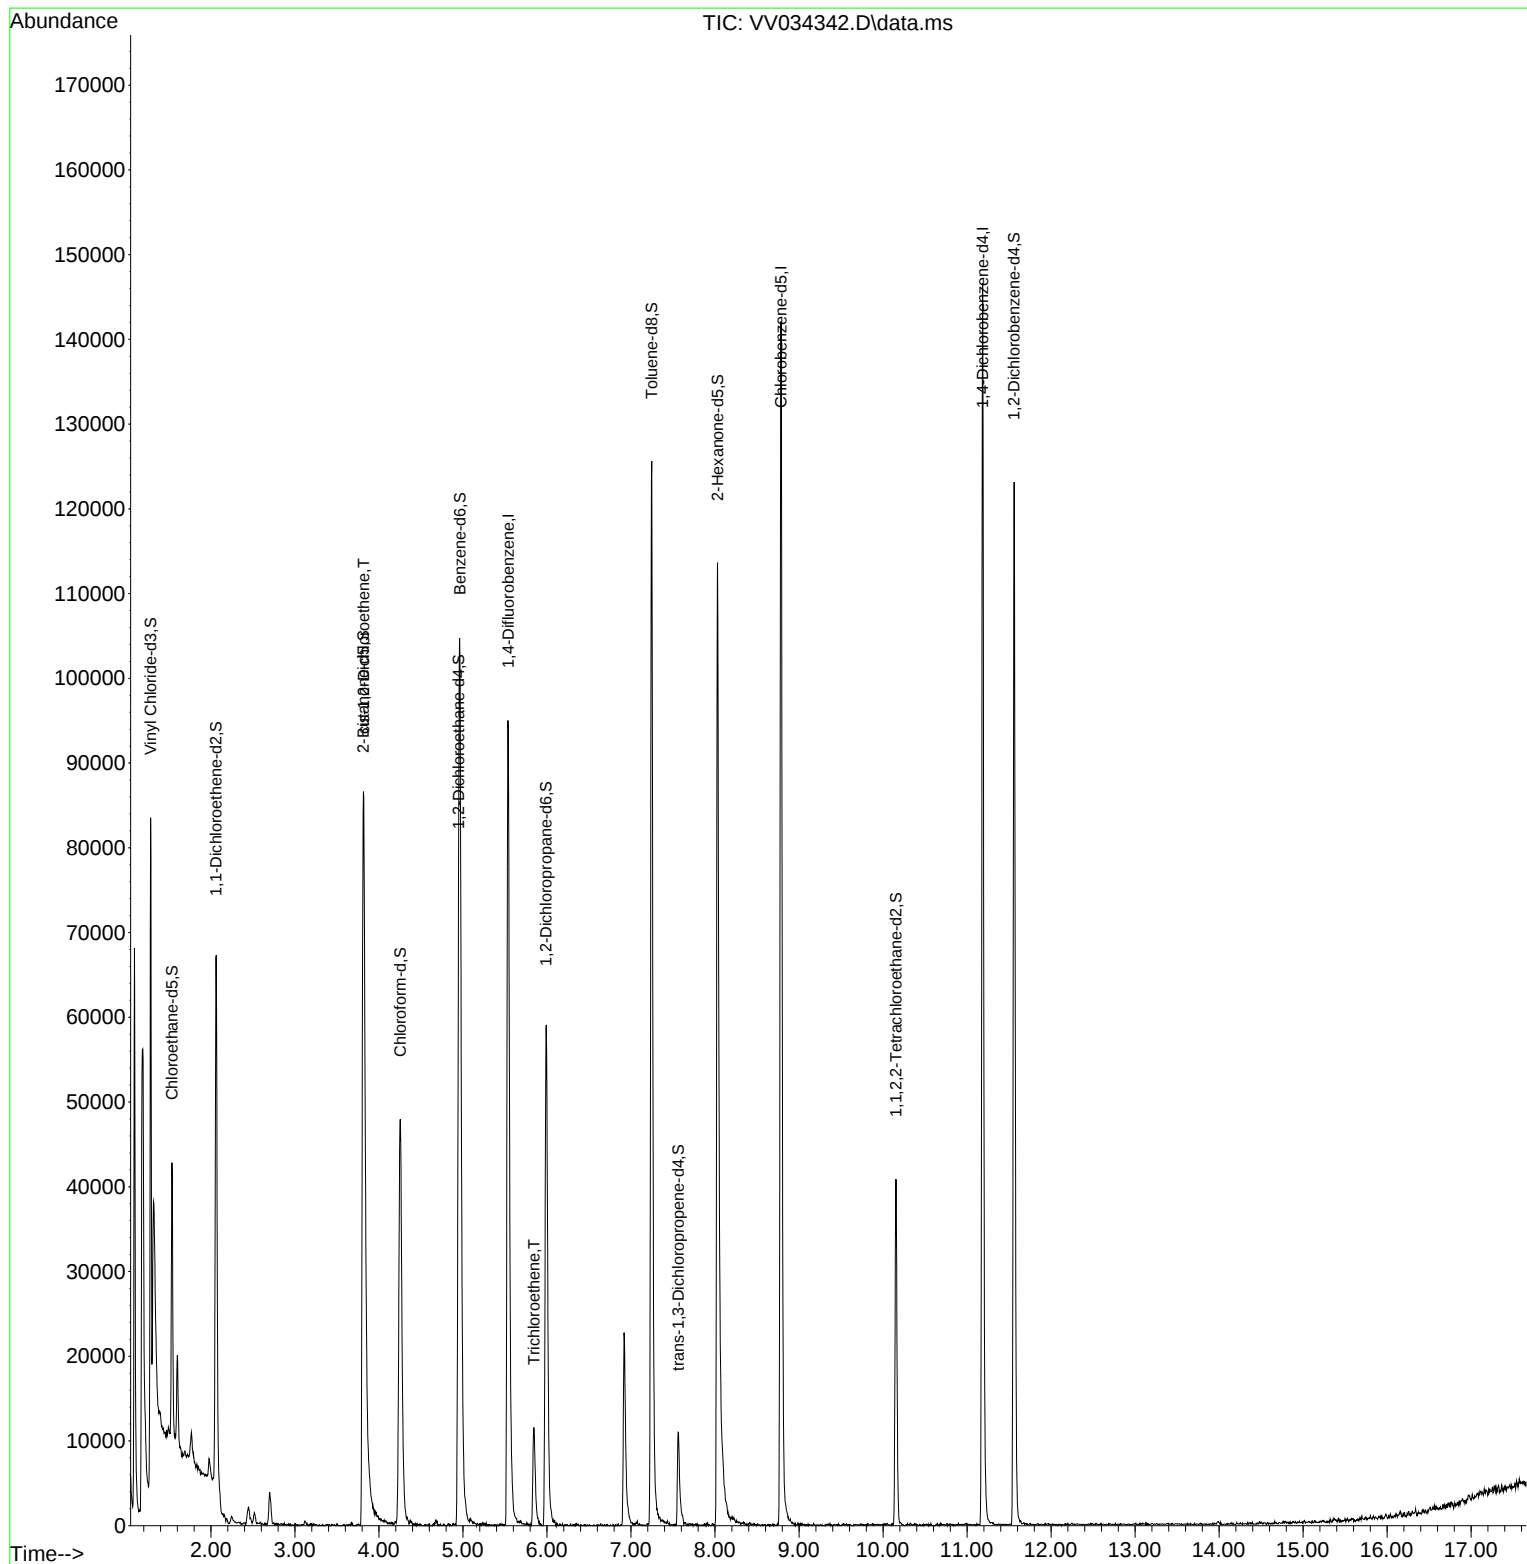


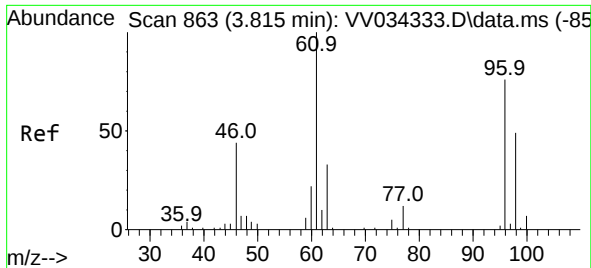

#22
cis-1,2-Dichloroethene
Concen: 5.229 ug/L
RT: 3.818 min Scan# 863
Delta R.T. 0.003 min
Lab File: VV034342.D
Acq: 22 Feb 2024 13:12

Instrument :
MSVOA_V
ClientSampleId :
C0AB7

Tgt Ion: 96 Resp: 35024
Ion Ratio Lower Upper
96 100
61 131.7 90.3 167.7
98 63.9 43.2 80.2

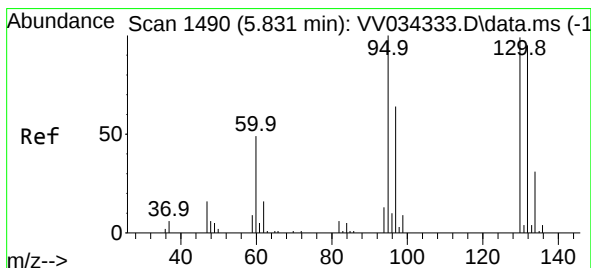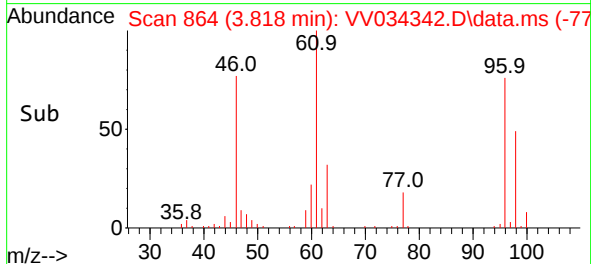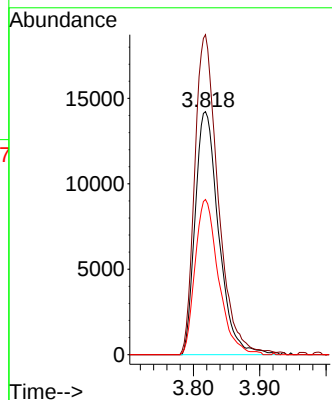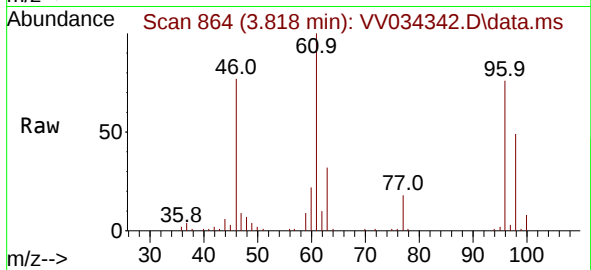

#34
Trichloroethene
Concen: 0.657 ug/L
RT: 5.844 min Scan# 1494
Delta R.T. 0.013 min
Lab File: VV034342.D
Acq: 22 Feb 2024 13:12

Tgt Ion: 95 Resp: 4453
Ion Ratio Lower Upper
95 100
97 60.6 45.1 83.7
132 100.5 66.0 122.6
130 94.3 72.2 134.0

