

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022224\
 Data File : VW034344.D
 Acq On : 22 Feb 2024 14:01
 Operator : SY/MD
 Sample : P1498-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE1

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 02/23/2024
 Supervised By :Semsettin Yesilyurt 02/23/2024

Quant Time: Feb 23 01:17:16 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 23 01:14:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	75234	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	69729	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	34024	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	18122	3.110	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	62.200%	
7) Chloroethane-d5	1.535	69	18094	3.545	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	71.000%	
11) 1,1-Dichloroethene-d2	2.060	65	9653	3.435	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	68.800%	
20) 2-Butanone-d5	3.809	46	48273	49.330	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	98.660%	
24) Chloroform-d	4.252	84	47977	4.531	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.600%	
26) 1,2-Dichloroethane-d4	4.947	65	24257	4.902	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	98.000%	
32) Benzene-d6	4.963	84	86348	4.127	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	82.600%	
36) 1,2-Dichloropropane-d6	5.992	67	25875	4.425	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	88.400%	
41) Toluene-d8	7.246	98	75012	3.901	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	78.000%	
43) trans-1,3-Dichloroprop...	7.561	79	7185	3.254	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	65.000%	
46) 2-Hexanone-d5	8.027	63	38098	48.331	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	96.660%	
56) 1,1,2,2-Tetrachloroeth...	10.152	84	17717	4.997	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	100.000%	
66) 1,2-Dichlorobenzene-d4	11.561	152	29234	4.724	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	94.400%	
Target Compounds						Qvalue
12) 1,1-Dichloroethene	2.069	96	6508	1.238	ug/L #	16
19) 1,1-Dichloroethane	3.117	63	8412	0.855	ug/L #	82
22) cis-1,2-Dichloroethene	3.818	96	22997	3.786	ug/L	97
25) Chloroform	4.278	83	11023	1.109	ug/L	97
29) 1,1,1-Trichloroethane	4.510	97	3369m	0.360	ug/L	
31) Carbon tetrachloride	4.735	117	18856	2.302	ug/L	99
34) Trichloroethene	5.834	95	36157	5.974	ug/L	96
47) Tetrachloroethene	7.905	164	16574	3.370	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022224\
Data File : VV034344.D
Acq On : 22 Feb 2024 14:01
Operator : SY/MD
Sample : P1498-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
C0AE1

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 02/23/2024
Supervised By :Semsettin Yesilyurt 02/23/2024


Quant Time: Feb 23 01:17:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 23 01:14:23 2024
Response via : Initial Calibration

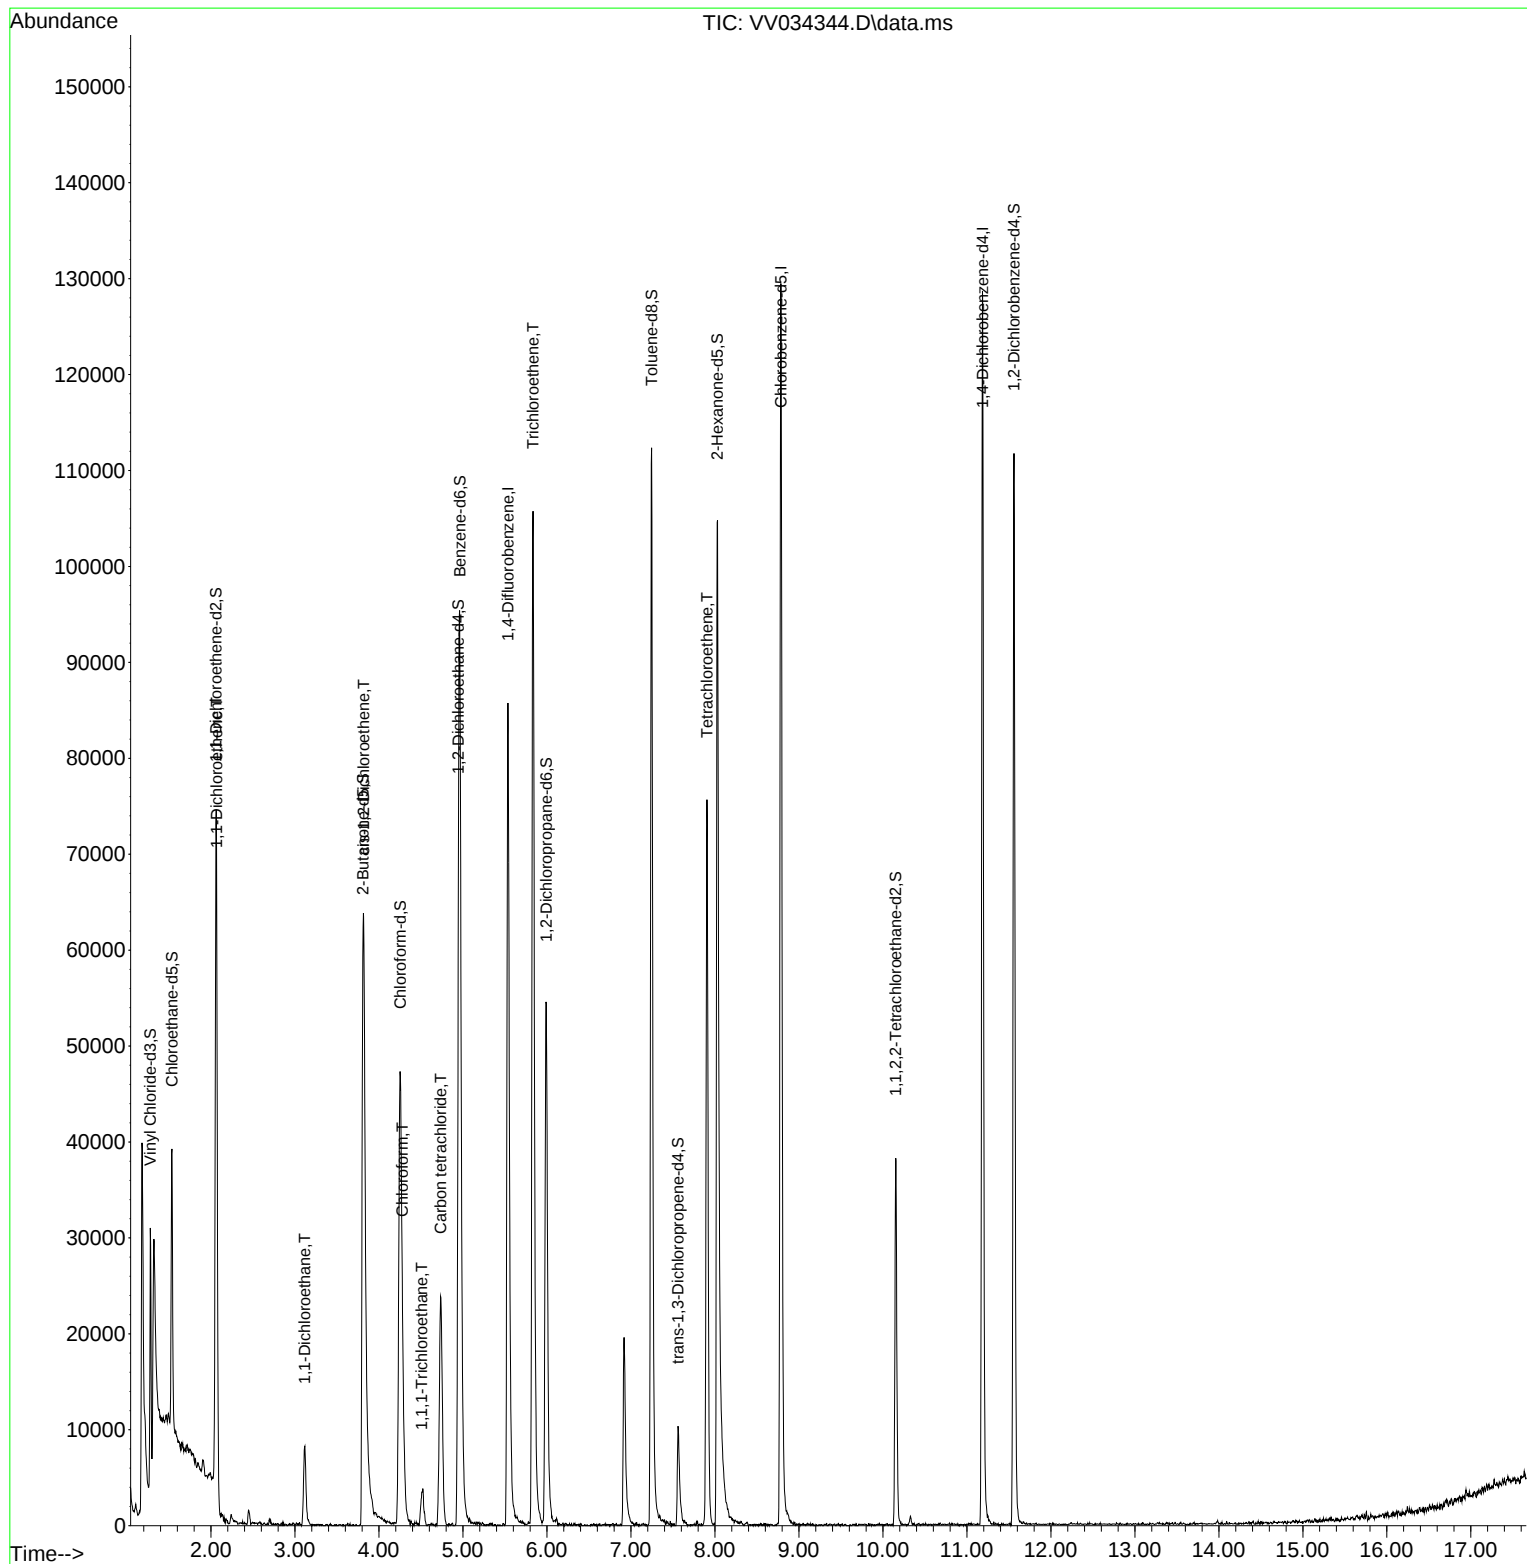

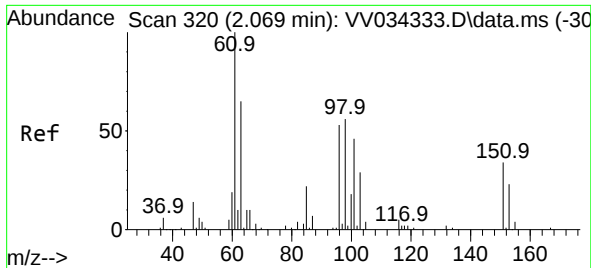

#12
1,1-Dichloroethene
Concen: 1.238 ug/L
RT: 2.069 min Scan# 31
Delta R.T. -0.000 min
Lab File: VV034344.D
Acq: 22 Feb 2024 14:01




Instrument :
MSVOA_V
ClientSampleId :
C0AE1

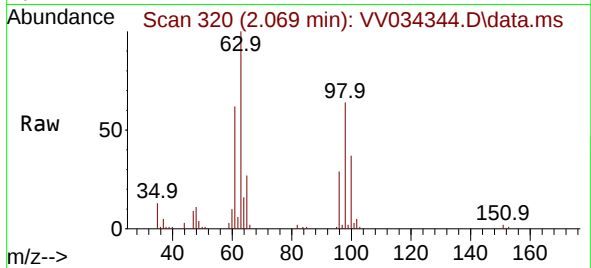


Tgt Ion: 96 Resp: 6508
Ion Ratio Lower Upper
96 100
61 213.1 128.8 239.2
63 343.0 97.9 181.9

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 02/23/2024
Supervised By :Semsettin Yesilyurt 02/23/2024

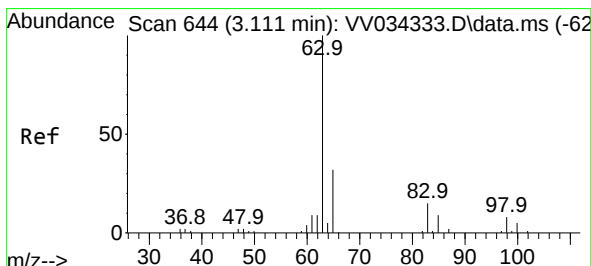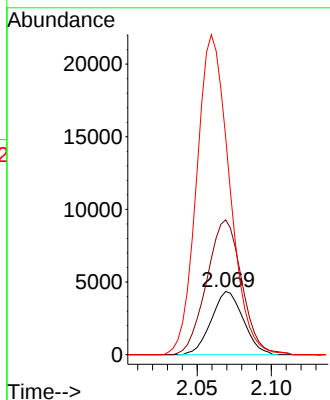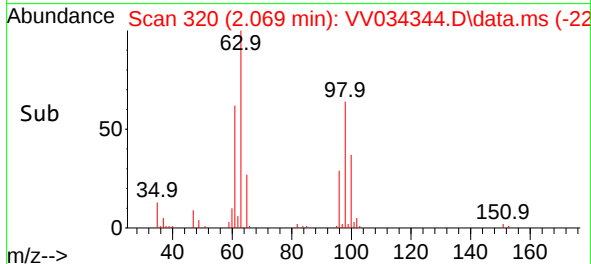


#19
1,1-Dichloroethane
Concen: 0.855 ug/L
RT: 3.117 min Scan# 646
Delta R.T. 0.006 min
Lab File: VV034344.D
Acq: 22 Feb 2024 14:01

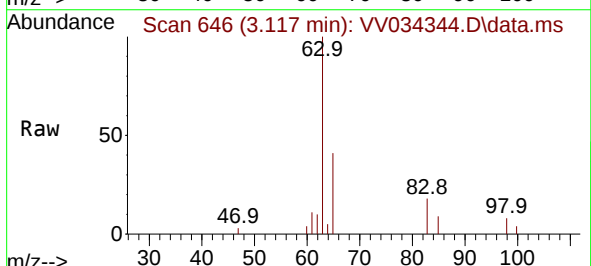

Tgt Ion: 63 Resp: 8412
Ion Ratio Lower Upper
63 100
65 41.0 20.8 38.6#
83 18.2 9.4 17.4#

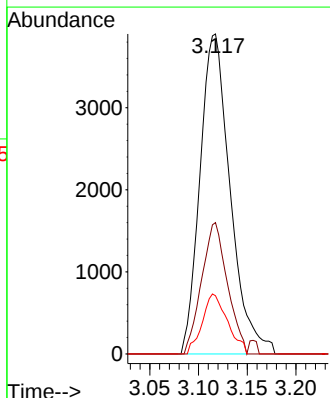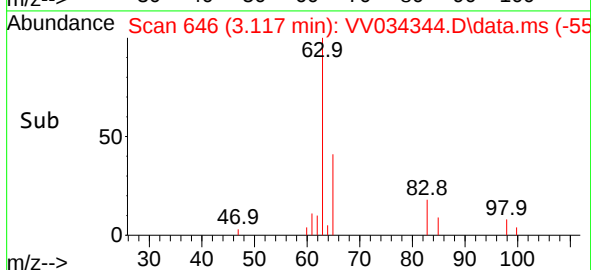

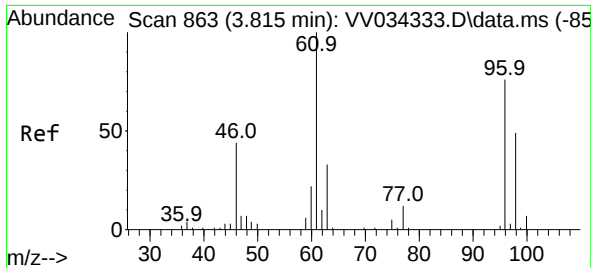





#22
cis-1,2-Dichloroethene
Concen: 3.786 ug/L
RT: 3.818 min Scan# 80
Delta R.T. 0.003 min
Lab File: VV034344.D
Acq: 22 Feb 2024 14:01

Instrument :
MSVOA_V
ClientSampleId :
C0AE1

Tgt Ion: 96 Resp: 2299
Ion Ratio Lower Upper
96 100
61 130.1 90.3 167.7
98 67.0 43.2 80.2




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 02/23/2024
Supervised By :Semsettin Yesilyurt 02/23/2024

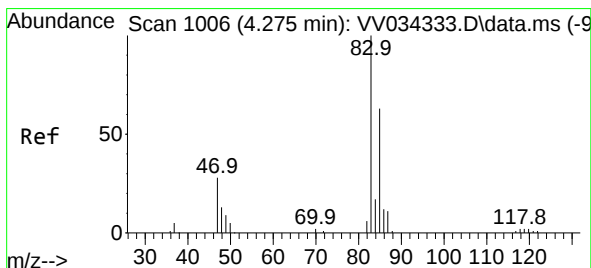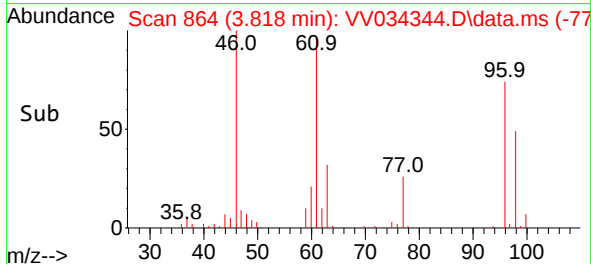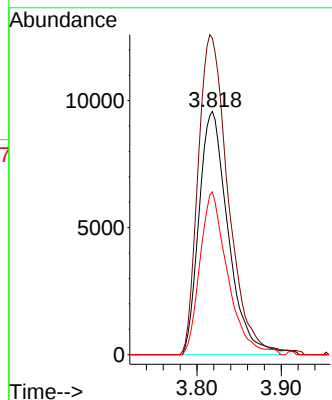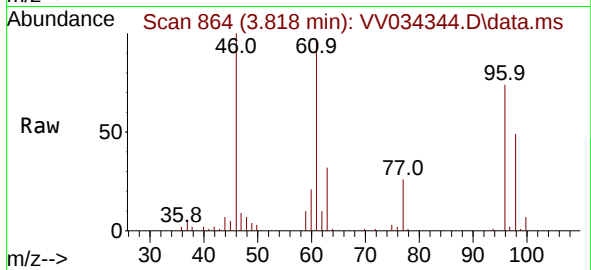

#25
Chloroform
Concen: 1.109 ug/L
RT: 4.278 min Scan# 1007
Delta R.T. 0.003 min
Lab File: VV034344.D
Acq: 22 Feb 2024 14:01


Tgt Ion: 83 Resp: 11023
Ion Ratio Lower Upper
83 100
85 65.1 47.5 88.1

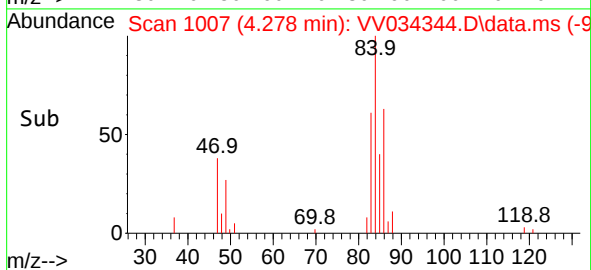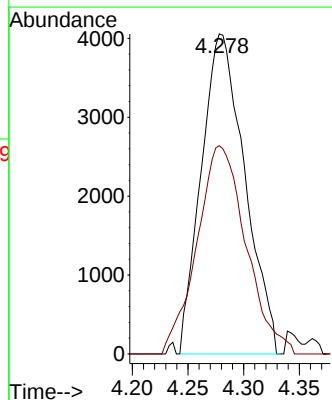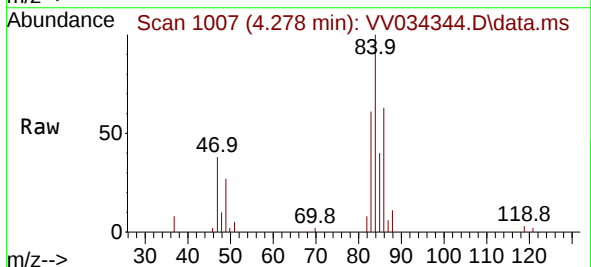

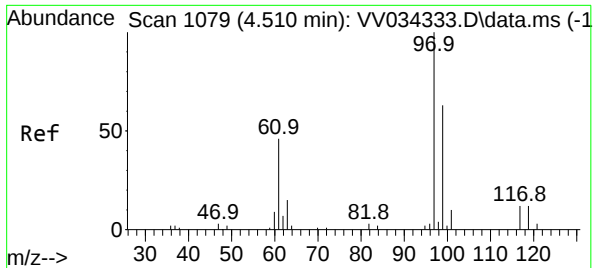

#29
1,1,1-Trichloroethane
Concen: 0.360 ug/L m
RT: 4.510 min Scan# 1079
Delta R.T. -0.000 min
Lab File: VV034344.D
Acq: 22 Feb 2024 14:01




Instrument :
MSVOA_V
ClientSampleId :
C0AE1

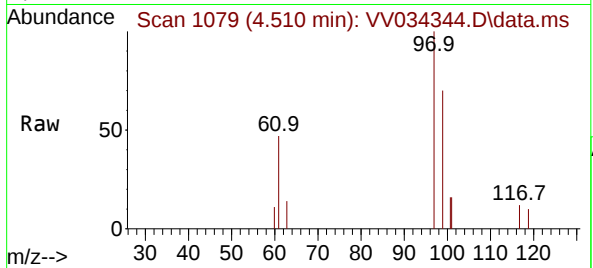

Tgt Ion: 97 Resp: 3369
Ion Ratio Lower Upper
97 100
99 64.9 50.6 75.8
61 47.1 36.8 55.2




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 02/23/2024
Supervised By :Semsettin Yesilyurt 02/23/2024

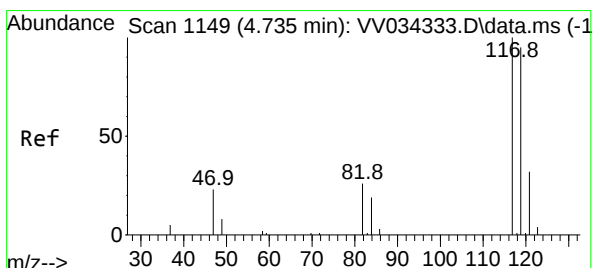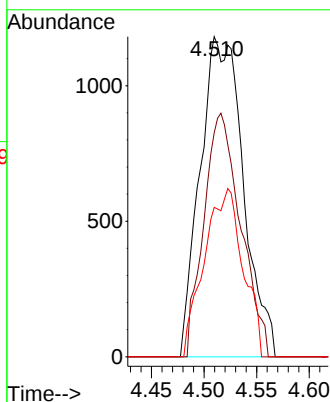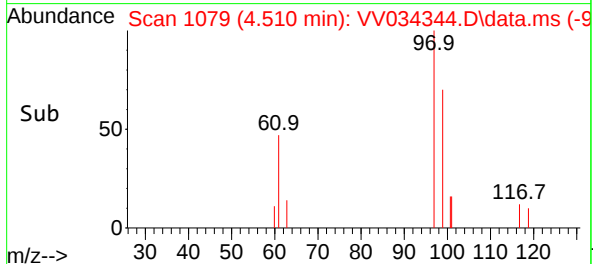

#31
Carbon tetrachloride
Concen: 2.302 ug/L
RT: 4.735 min Scan# 1149
Delta R.T. -0.000 min
Lab File: VV034344.D
Acq: 22 Feb 2024 14:01


Tgt Ion:117 Resp: 18856
Ion Ratio Lower Upper
117 100
119 94.5 76.1 114.1

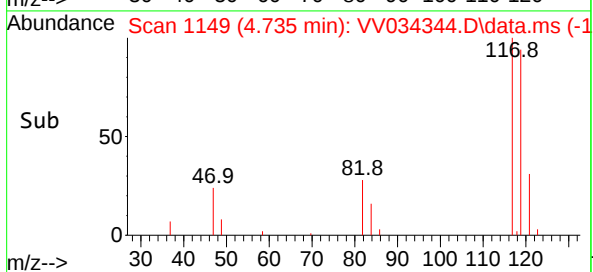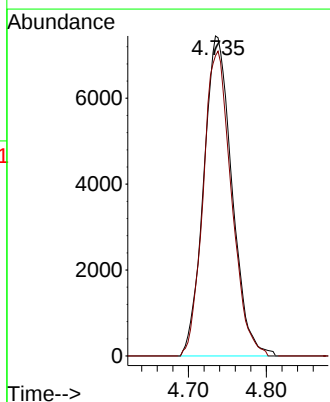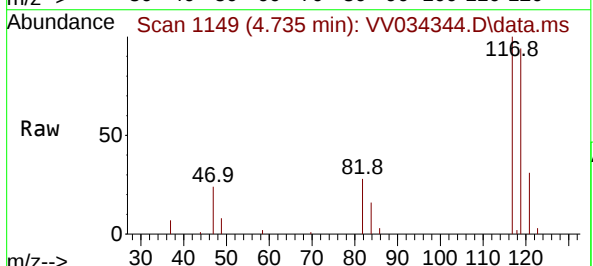

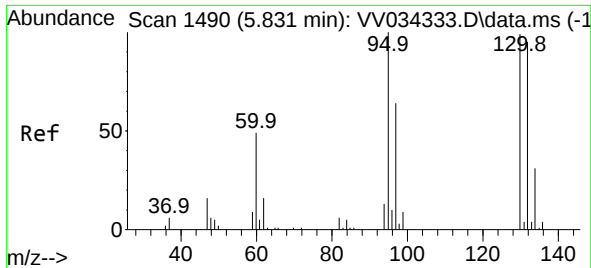

#34
Trichloroethene
Concen: 5.974 ug/L
RT: 5.834 min Scan# 1490
Delta R.T. 0.003 min
Lab File: VV034344.D
Acq: 22 Feb 2024 14:01




Instrument :
MSVOA_V
ClientSampleId :
C0AE1

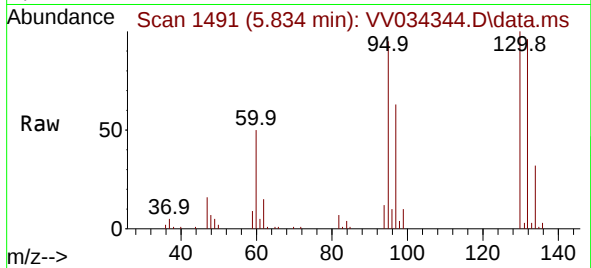


Tgt Ion: 95 Resp: 3615
Ion Ratio Lower Upper
95 100
97 67.0 45.1 83.7
132 101.2 66.0 122.6
130 105.6 72.2 134.0

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 02/23/2024
Supervised By :Semsettin Yesilyurt 02/23/2024

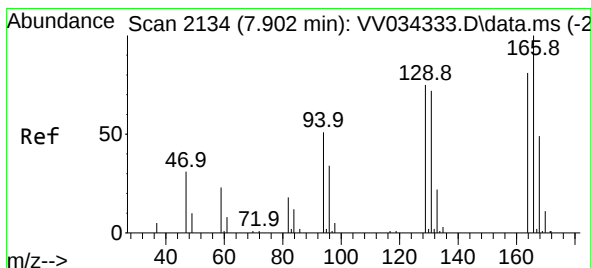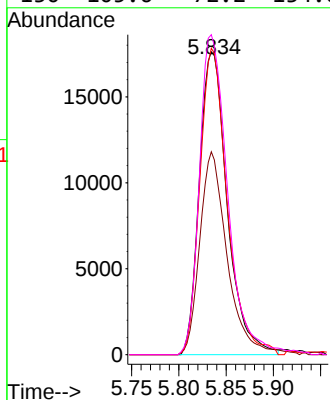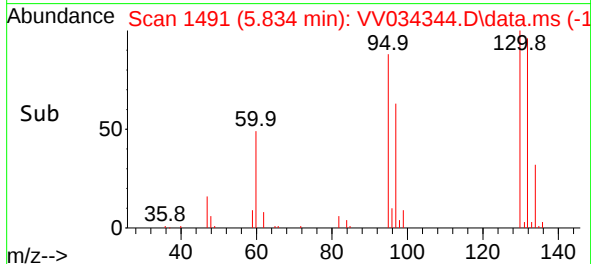

#47
Tetrachloroethene
Concen: 3.370 ug/L
RT: 7.905 min Scan# 2135
Delta R.T. 0.003 min
Lab File: VV034344.D
Acq: 22 Feb 2024 14:01

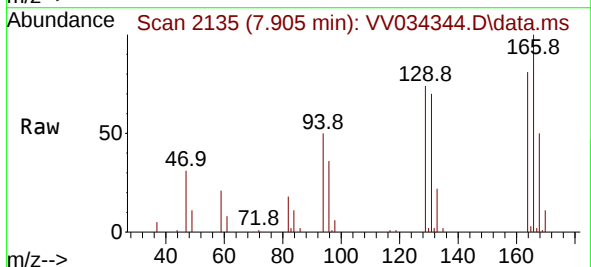

Tgt Ion:164 Resp: 16574
Ion Ratio Lower Upper
164 100
129 91.7 67.8 125.8
131 86.3 63.0 117.0
166 123.3 92.6 172.0

