

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022321\
 Data File : VV020376.D
 Acq On : 23 Feb 2021 10:34
 Operator : SY/MD
 Sample : VV0223WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK32

Quant Time: Feb 24 01:23:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Feb 24 01:23:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	296359	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	287359	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.255	152	136698	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	96566	4.63	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.60%
7) Chloroethane-d5	1.567	69	79177	4.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.60%
11) 1,1-Dichloroethene-d2	2.108	63	132656	3.26	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.20%
20) 2-Butanone-d5	3.905	46	173910	48.11	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.22%
24) Chloroform-d	4.355	84	170765	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.60%
26) 1,2-Dichloroethane-d4	5.037	65	87752	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
32) Benzene-d6	5.053	84	350260	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.40%
36) 1,2-Dichloropropane-d6	6.075	67	104022	4.88	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.60%
41) Toluene-d8	7.320	98	317169	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.40%
45) trans-1,3-Dichloroprop...	7.628	79	34991	4.30	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.00%
48) 2-Hexanone-d5	8.095	63	119420	41.83	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.66%
59) 1,1,2,2-Tetrachloroeth...	10.223	84	66235	4.37	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.40%
65) 1,2-Dichlorobenzene-d4	11.631	152	126102	5.20	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.00%
Target Compounds						
50) 2-Hexanone	8.146	43	14482	1.68	ug/L	Qvalue # 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022321\
Data File : VV020376.D
Acq On : 23 Feb 2021 10:34
Operator : SY/MD
Sample : VV0223WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK32

Quant Time: Feb 24 01:23:47 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Feb 24 01:23:15 2021
Response via : Initial Calibration

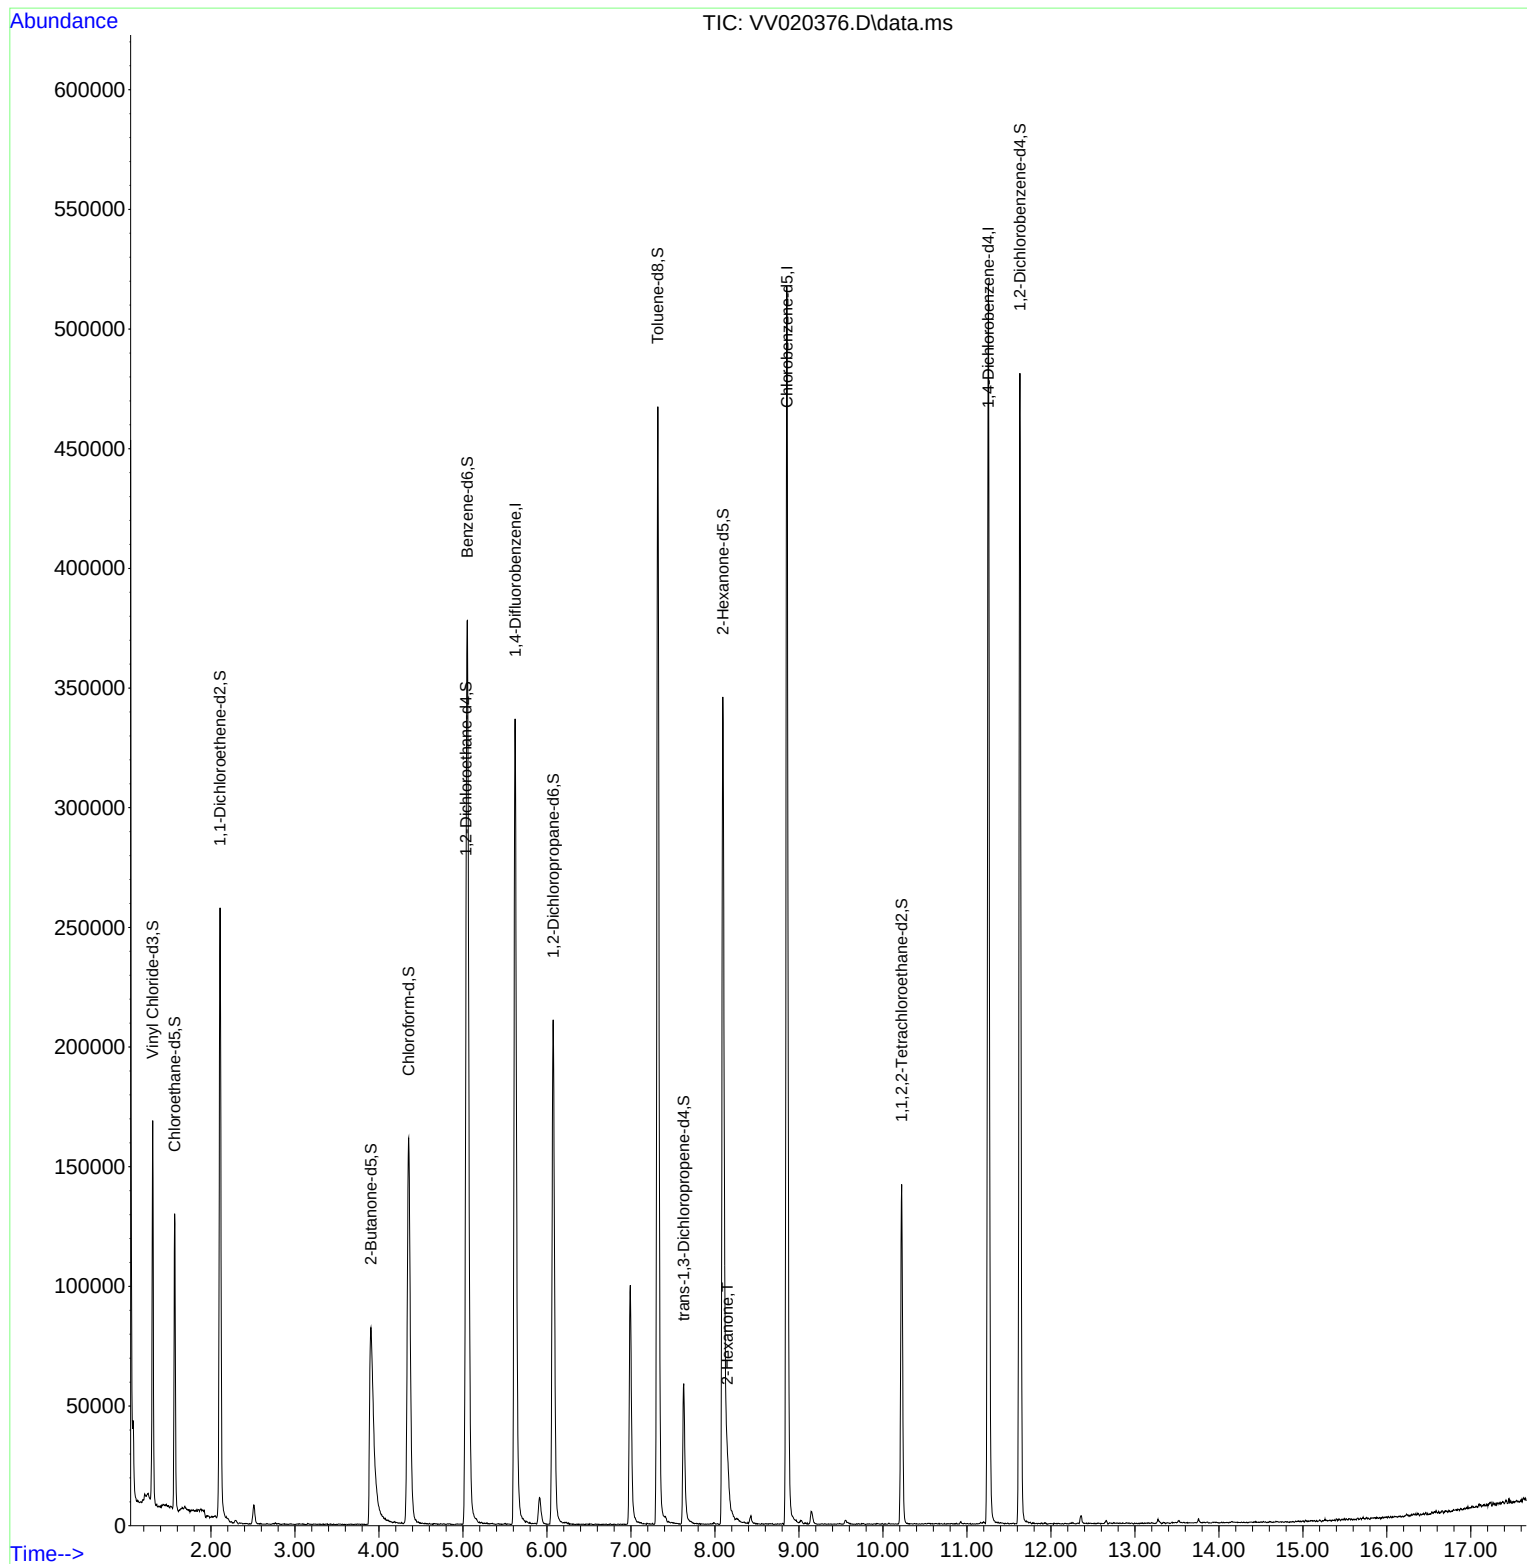

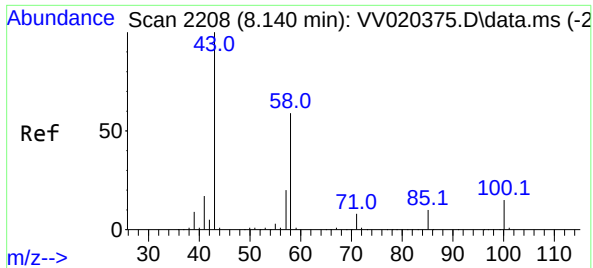

#50
2-Hexanone
Concen: 1.68 ug/L
RT: 8.146 min Scan# 2210
Delta R.T. 0.006 min
Lab File: VV020376.D
Acq: 23 Feb 2021 10:34

Instrument :
MSVOA_V
ClientSampleId :
VBLK32

Tgt Ion: 43	Resp: 14482
Ion Ratio	Lower Upper
43	100
58	48.7 41.6 62.4
57	12.7 15.4 23.0#
100	10.8 11.2 16.8#

