

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022321\
 Data File : VV020376.D
 Acq On : 23 Feb 2021 10:34
 Operator : SY/MD
 Sample : VV0223WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK32

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC: VV020376.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	95	rVB	160787	170441	18.02%	2.142%
2	1.568	157	164	178	rVB	124504	140807	14.89%	1.770%
3	2.108	320	332	354	rBV	254883	369284	39.04%	4.641%
4	2.510	446	457	472	rBV2	7974	14037	1.48%	0.176%
5	3.905	879	891	934	rBV	82290	297189	31.42%	3.735%
6	4.355	1010	1031	1055	rBV	161190	408128	43.15%	5.129%
7	5.053	1228	1248	1281	rBV2	377714	945793	100.00%	11.887%
8	5.622	1410	1425	1452	rBV	336643	679054	71.80%	8.534%
9	5.911	1504	1515	1532	rBV4	11083	24787	2.62%	0.312%
10	6.075	1552	1566	1593	rBV	210721	434358	45.93%	5.459%
11	6.992	1839	1851	1878	rBV	99916	185910	19.66%	2.337%
12	7.320	1941	1953	1976	rBV	467018	822062	86.92%	10.332%
13	7.628	2037	2049	2071	rBV2	58773	106806	11.29%	1.342%
14	8.095	2179	2194	2239	rBV2	345834	727972	76.97%	9.149%
15	8.857	2420	2431	2464	rBV	517411	840138	88.83%	10.559%
16	9.146	2510	2521	2537	rBV4	5263	10446	1.10%	0.131%
17	10.223	2843	2856	2875	rBV	141941	221726	23.44%	2.787%
18	11.255	3166	3177	3203	rBV	518169	804753	85.09%	10.114%
19	11.631	3281	3294	3317	rBV	480733	752924	79.61%	9.463%




Sum of corrected areas: 7956615

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022321\
Data File : VV020376.D
Acq On : 23 Feb 2021 10:34
Operator : SY/MD
Sample : VV0223WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

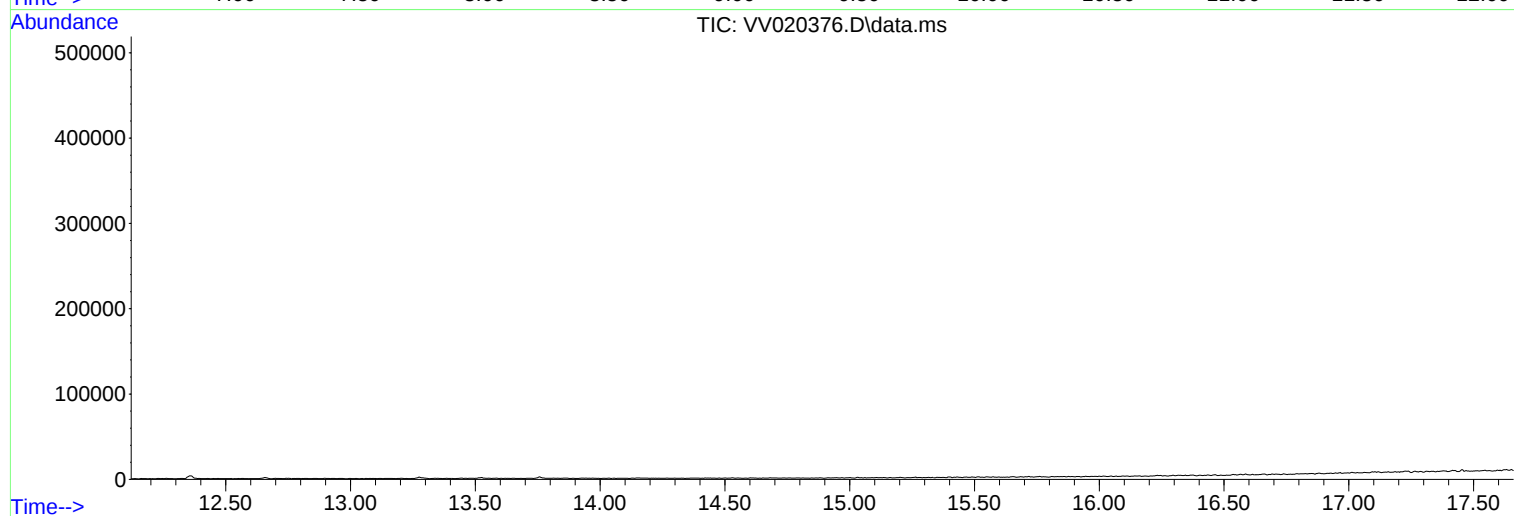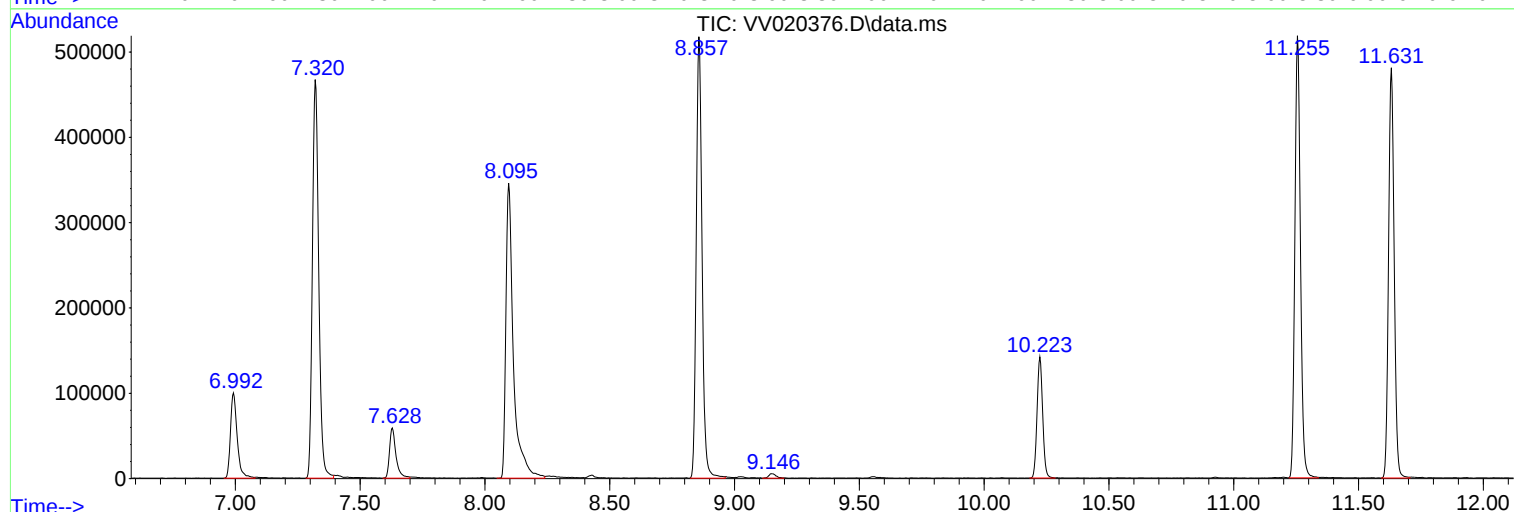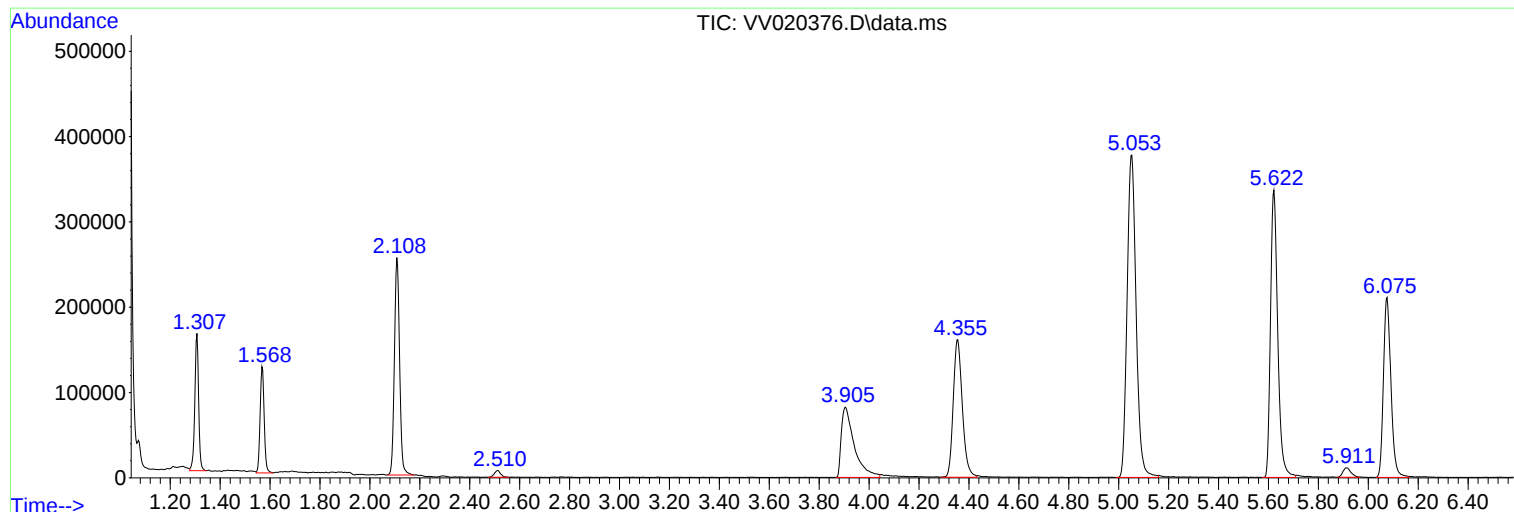

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022321\
Data File : VV020376.D
Acq On : 23 Feb 2021 10:34
Operator : SY/MD
Sample : VV0223WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022321\
Data File : VV020376.D
Acq On : 23 Feb 2021 10:34
Operator : SY/MD
Sample : VV0223WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
