
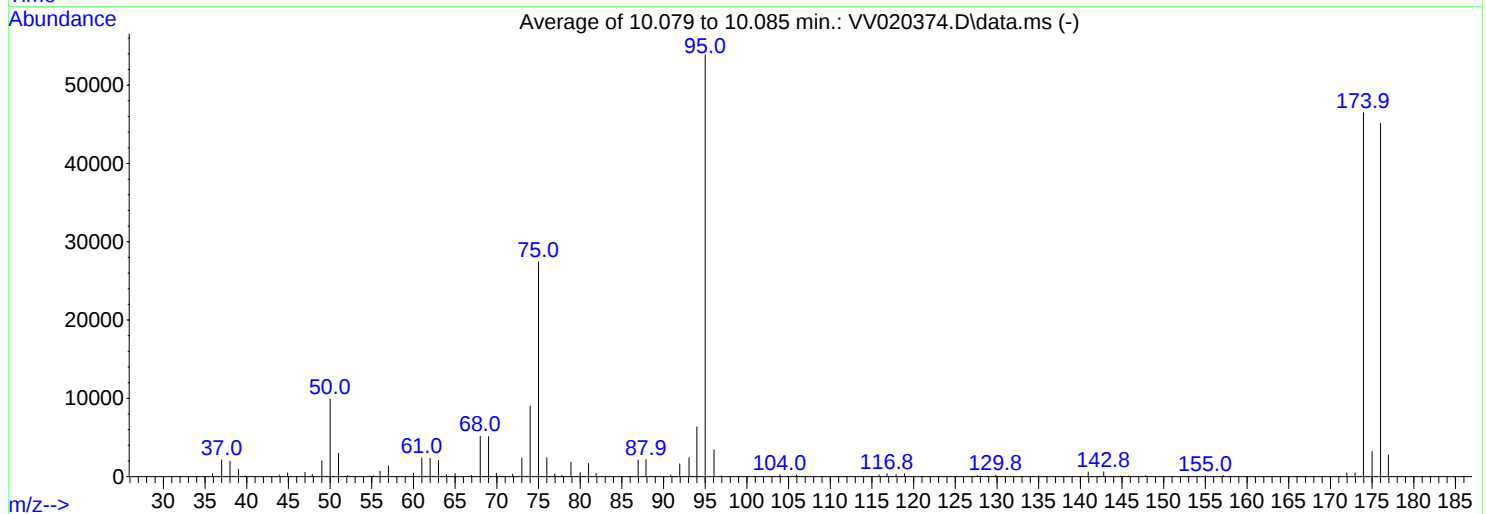


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022321\
 Data File : VV020374.D
 Acq On : 23 Feb 2021 08:55
 Operator : SY/MD
 Sample : BFB32
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB32

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Feb 24 01:23:15 2021

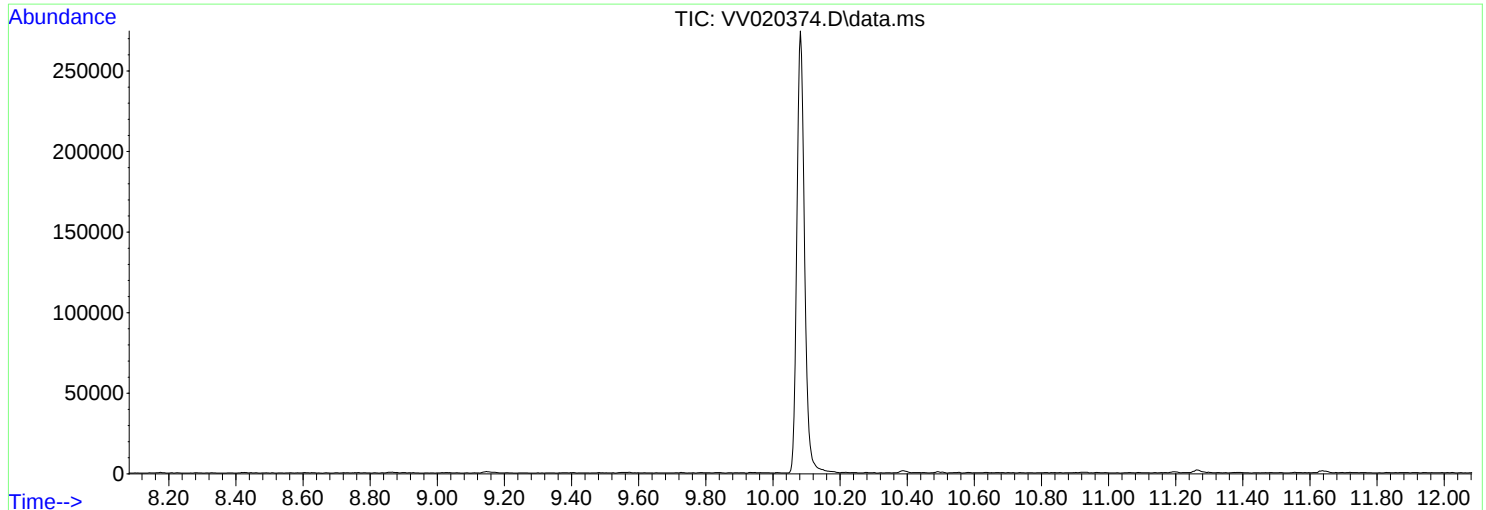

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	9908	PASS
75	95	30	80	50.9	27416	PASS
95	95	100	100	100.0	53872	PASS
96	95	5	9	6.4	3445	PASS
173	174	0.00	2	1.1	501	PASS
174	95	50	120	86.3	46501	PASS
175	174	5	9	6.9	3212	PASS
176	174	95	101	97.1	45133	PASS
177	176	5	9	6.1	2770	PASS

m/z	Abundance
35.90	440.0
37.00	2225.0
38.00	1831.0
39.00	866.0
39.80	245.0
44.00	605.0
44.90	506.0
46.10	112.0
47.00	667.0
47.90	307.0
49.00	1930.0
50.00	10144.0
51.00	3215.0
52.10	200.0
54.80	139.0
55.20	113.0
56.00	695.0
57.00	1534.0
60.00	530.0
61.00	2420.0
62.00	2363.0
63.00	2094.0
64.00	240.0
65.00	366.0
66.90	123.0
68.00	5170.0
69.00	5113.0
70.00	443.0
71.90	339.0
73.00	2526.0
74.00	8981.0
75.00	27608.0
76.00	2603.0
76.90	321.0
77.70	154.0
78.90	1814.0
80.00	539.0
81.00	1761.0
81.90	419.0
87.00	2056.0
87.90	2113.0
90.80	240.0
92.00	1514.0
93.10	2446.0
94.00	6473.0
95.00	53192.0
96.00	3610.0
96.90	127.0
103.90	232.0
104.90	124.0
105.90	214.0
115.90	219.0
116.80	371.0
118.00	276.0
118.90	374.0
127.60	135.0
128.00	167.0
129.90	195.0
135.00	122.0
137.00	113.0
141.00	513.0
142.80	569.0
144.80	131.0
147.80	121.0
154.90	142.0
157.10	168.0
171.90	382.0
173.00	434.0
174.00	44768.0
175.00	3140.0
176.00	43616.0
176.90	2612.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

m/z	Abundance
35.90	448.0
37.00	2233.0
38.00	2089.0
39.00	970.0
39.80	277.0
44.00	613.0
44.90	508.0
47.00	560.0
47.90	304.0
49.00	2091.0
50.00	10307.0
51.00	3108.0
52.10	159.0
54.80	137.0
55.20	130.0
56.00	688.0
57.00	1422.0
60.00	465.0
61.00	2485.0
62.00	2379.0
63.00	2110.0
63.90	247.0
65.00	387.0
67.00	137.0
68.00	5334.0
69.00	5236.0
69.90	452.0
71.90	357.0
73.00	2422.0
74.00	9322.0
75.00	28336.0
76.00	2514.0
76.90	351.0
77.80	178.0
78.90	1910.0
80.00	553.0
81.00	1732.0
81.90	419.0
86.90	2197.0
87.90	2248.0
90.80	213.0
92.00	1749.0
93.10	2509.0
94.00	6480.0
95.00	55752.0
96.00	3523.0
96.90	152.0
103.90	260.0
104.90	117.0
106.00	216.0
115.80	209.0
116.80	414.0
117.90	263.0
118.90	393.0
127.60	188.0
128.80	102.0
129.80	187.0
135.00	137.0
137.10	103.0
141.00	604.0
142.80	623.0
144.90	116.0
145.80	129.0
147.80	166.0
155.00	151.0
157.20	167.0
171.10	123.0
172.00	470.0
172.90	519.0
173.90	48128.0
175.00	3347.0
176.00	46632.0
176.90	2840.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

m/z	Abundance
35.90	360.0
37.00	1928.0
38.00	2106.0
39.00	971.0
39.80	284.0
43.90	619.0
44.90	429.0
47.00	430.0
47.80	266.0
49.00	2032.0
50.00	9273.0
51.00	2675.0
52.10	115.0
55.20	151.0
56.00	730.0
57.00	1182.0
60.00	446.0
61.00	2278.0
62.00	2270.0
63.00	1989.0
63.90	241.0
65.00	405.0
67.00	173.0
68.00	4991.0
69.00	4962.0
69.90	411.0
71.90	298.0
73.00	2177.0
74.00	8720.0
75.00	26304.0
76.00	2168.0
77.00	345.0
77.90	214.0
78.90	1773.0
80.00	495.0
81.00	1514.0
81.90	375.0
85.80	108.0
86.90	2176.0
87.90	2188.0
90.90	172.0
91.90	1660.0
93.00	2366.0
94.00	6121.0
95.00	52672.0
96.10	3203.0
104.00	286.0
106.00	180.0
115.80	198.0
116.80	413.0
117.80	239.0
118.90	354.0
127.70	187.0
128.90	114.0
129.80	197.0
135.00	124.0
140.90	667.0
142.80	662.0
145.80	156.0
147.80	152.0
155.10	161.0
157.20	113.0
172.00	593.0
172.90	551.0
173.90	46608.0
175.00	3150.0
176.00	45152.0
177.00	2859.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

m/z	Abundance
39.90	169.0
43.90	406.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32