


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022323\
Data File : VV030083.D
Acq On : 23 Feb 2023 09:35
Operator : SY/MD
Sample : BFB223
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB223

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Feb 23 21:31:17 2023

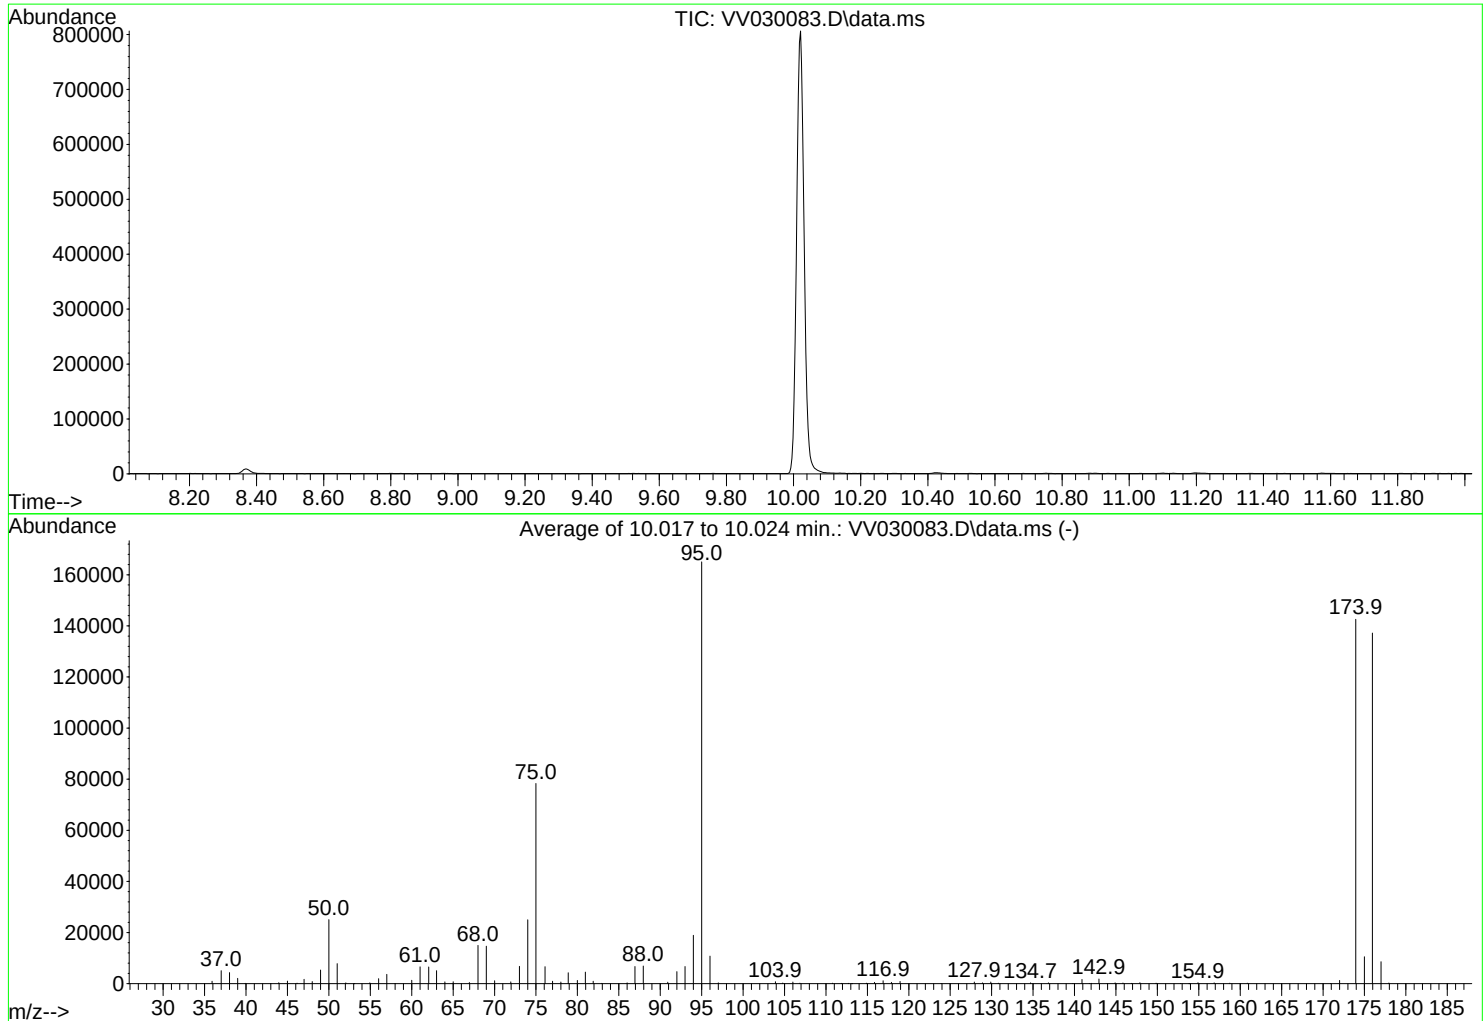

AutoFind: Scans 2792, 2793, 2794; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	25053	PASS
75	95	30	80	47.4	78301	PASS
95	95	100	100	100.0	165056	PASS
96	95	5	9	6.5	10776	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.4	142592	PASS
175	174	5	9	7.4	10522	PASS
176	174	95	105	96.2	137152	PASS
177	176	5	10	6.2	8566	PASS

m/z	Abundance
39.90	100.0
44.00	454.0

Instrument :
MSVOA_V
ClientSampleId :
BFB223

m/z	Abundance
35.90	1054.0
37.00	5233.0
38.00	4465.0
39.00	2070.0
39.90	265.0
43.00	105.0
44.00	821.0
45.00	940.0
46.20	180.0
47.00	1741.0
48.00	852.0
49.00	5406.0
50.00	25784.0
51.00	8090.0
52.10	364.0
53.00	104.0
55.00	302.0
56.00	2064.0
57.00	3911.0
58.00	126.0
60.00	1328.0
61.00	6713.0
62.00	6793.0
63.00	5192.0
64.00	710.0
65.00	818.0
67.00	473.0
68.00	15305.0
69.00	15205.0
70.00	1138.0
72.00	750.0
73.00	6785.0
74.00	25616.0
75.00	79792.0
76.10	6873.0
77.00	978.0
78.00	630.0
78.90	4287.0
80.00	1332.0
81.00	4657.0
81.90	905.0
83.00	114.0
86.00	305.0
87.00	6814.0
87.90	7094.0
90.90	576.0
92.00	4787.0
93.00	6789.0
94.00	18952.0
95.00	166400.0
96.00	11019.0
97.00	320.0
103.90	773.0
104.80	202.0
106.00	645.0
106.90	171.0
110.80	153.0
111.80	123.0
112.70	125.0
114.90	212.0
115.90	521.0
116.90	1088.0
117.90	549.0
119.00	827.0
123.90	113.0
127.90	620.0
128.90	281.0
129.90	592.0
130.80	182.0
134.70	373.0
136.80	275.0
139.80	105.0
140.90	1661.0
142.00	219.0
142.90	1858.0
143.90	115.0
144.90	386.0
145.90	188.0
146.90	135.0
147.90	385.0
149.80	158.0
154.90	413.0
156.80	333.0
158.80	256.0
160.90	209.0
170.90	127.0
172.00	1275.0
174.00	141952.0
175.00	10565.0
175.90	134912.0
177.00	8620.0
177.90	262.0

Instrument :
MSVOA_V
ClientSampleId :
BFB223

m/z	Abundance
35.90	963.0
37.00	5226.0
38.00	4509.0
39.00	2112.0
40.00	255.0
43.00	105.0
43.90	825.0
45.00	1012.0
46.20	192.0
47.00	1747.0
48.00	869.0
49.00	5520.0
50.00	26072.0
51.00	8101.0
52.00	353.0
54.90	321.0
56.00	2017.0
57.00	3714.0
58.00	109.0
60.00	1379.0
61.00	6768.0
62.00	6687.0
63.00	5251.0
64.00	703.0
65.00	747.0
66.90	454.0
68.00	15444.0
69.00	15002.0
70.00	1196.0
71.90	691.0
73.00	7018.0
74.00	25936.0
75.00	81040.0
76.10	6890.0
77.00	942.0
78.00	665.0
78.90	4433.0
80.00	1280.0
80.90	4655.0
81.90	974.0
82.90	101.0
86.00	341.0
87.00	6888.0
87.90	7166.0
90.90	574.0
92.00	4884.0
93.00	6881.0
94.00	19512.0
95.00	170816.0
96.00	11146.0
97.00	341.0
103.90	790.0
104.80	251.0
106.00	619.0
106.90	182.0
110.80	163.0
111.90	133.0
112.70	147.0
114.90	218.0
115.90	484.0
116.90	1163.0
117.90	536.0
118.90	882.0
123.90	122.0
127.90	640.0
128.90	316.0
129.90	607.0
130.80	229.0
134.70	370.0
136.90	330.0
139.80	101.0
140.90	1635.0
142.10	200.0
143.00	1909.0
144.00	115.0
144.90	348.0
145.90	224.0
146.90	144.0
147.90	370.0
149.90	161.0
152.80	130.0
154.90	398.0
156.80	292.0
158.80	210.0
160.90	211.0
170.90	106.0
172.00	1306.0
174.00	147648.0
175.00	10908.0
176.00	141888.0
177.00	8805.0
177.90	299.0

Instrument :
MSVOA_V
ClientSampleId :
BFB223

m/z	Abundance
35.90	802.0
37.00	4695.0
38.00	4101.0
39.00	1957.0
40.00	232.0
43.90	823.0
45.00	976.0
46.00	142.0
47.00	1681.0
48.00	762.0
49.00	5080.0
50.00	23304.0
51.00	7248.0
52.00	292.0
55.00	334.0
56.00	1811.0
57.00	3206.0
60.00	1241.0
61.00	6206.0
62.10	6154.0
63.00	4705.0
64.00	659.0
65.00	640.0
66.90	399.0
68.00	14124.0
69.00	13743.0
70.00	1163.0
72.00	625.0
73.00	6560.0
74.00	23432.0
75.00	74072.0
76.10	6195.0
77.00	920.0
78.00	672.0
78.90	4149.0
80.00	1124.0
80.90	4167.0
81.90	931.0
82.90	101.0
86.00	321.0
86.90	6365.0
88.00	6518.0
90.90	534.0
92.00	4492.0
93.00	6382.0
94.00	18176.0
95.00	157952.0
96.00	10163.0
97.00	325.0
103.90	737.0
104.80	277.0
106.00	554.0
106.80	198.0
110.80	164.0
111.80	132.0
112.70	134.0
113.10	110.0
114.90	195.0
115.80	453.0
116.90	1114.0
117.90	505.0
118.90	839.0
127.90	631.0
128.90	302.0
129.90	600.0
130.80	243.0
134.70	260.0
136.90	387.0
140.90	1533.0
141.80	207.0
143.00	1730.0
144.90	277.0
145.80	285.0
146.90	138.0
147.90	372.0
149.90	165.0
152.80	151.0
153.80	106.0
154.90	395.0
156.90	286.0
158.70	164.0
160.80	208.0
172.00	1192.0
173.90	138176.0
175.00	10092.0
176.00	134656.0
177.00	8272.0
178.00	272.0

Instrument :
MSVOA_V
ClientSampleId :
BFB223