




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022324\
Data File : VV034376.D
Acq On : 23 Feb 2024 15:22
Operator : SY/MD
Sample : P1566-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JWAD2

Manual IntegrationsAPPROVED

Quant Time: Feb 24 00:48:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Feb 24 00:41:32 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/27/2024
Supervised By :Semsettin Yesilyurt 02/27/2024

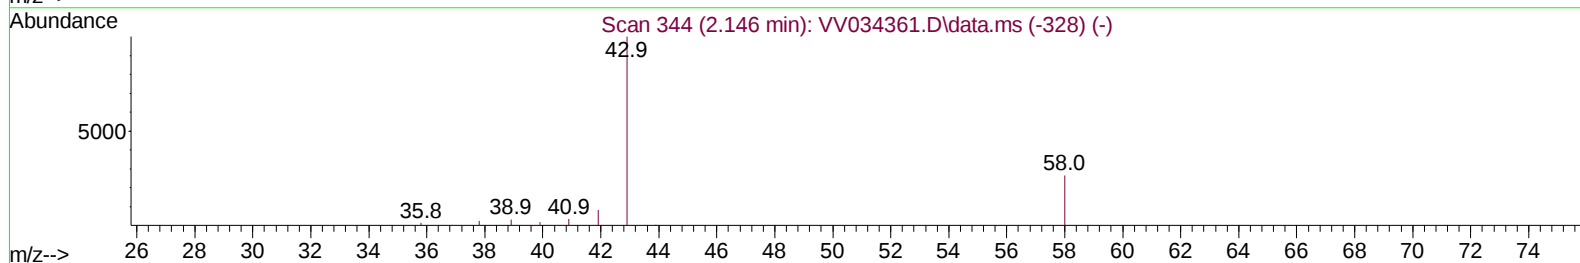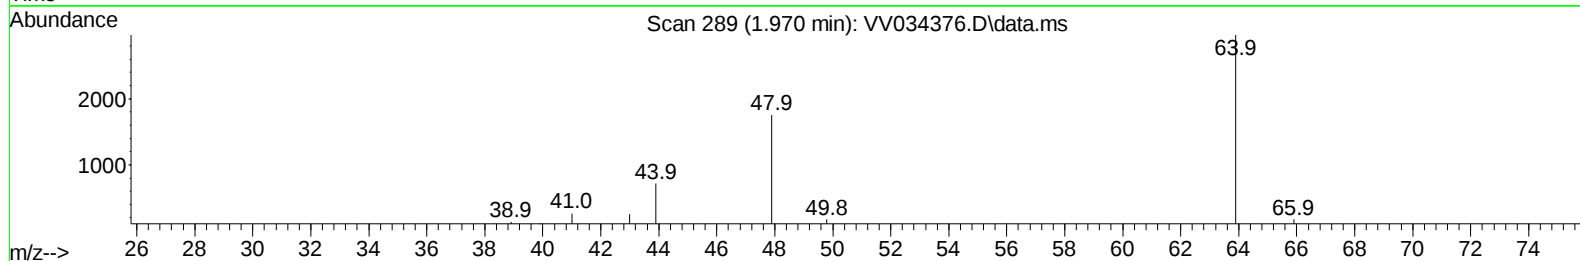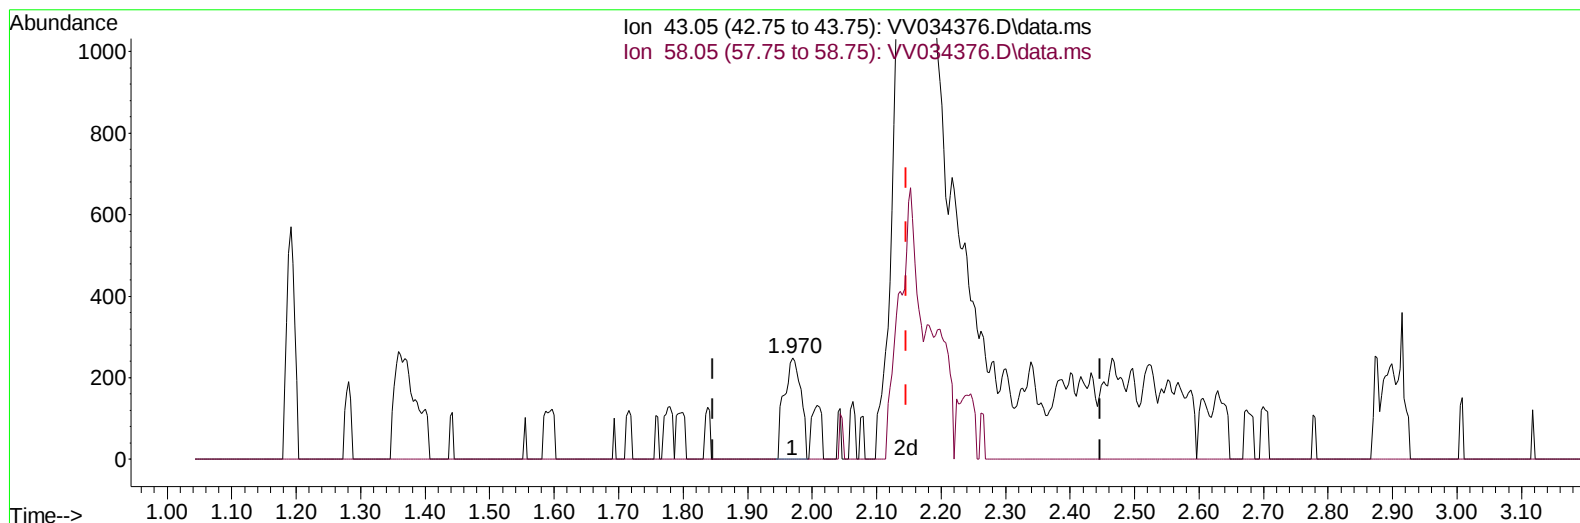

TIC: VV034376.D\data.ms

(13) Acetone (T)

1.970min (-0.177) 0.57 ug/L

response 449

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	6.90	9.13
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022324\
Data File : VV034376.D
Acq On : 23 Feb 2024 15:22
Operator : SY/MD
Sample : P1566-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JWAD2

Manual IntegrationsAPPROVED

Quant Time: Feb 24 00:48:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Feb 24 00:41:32 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/27/2024
Supervised By :Semsettin Yesilyurt 02/27/2024

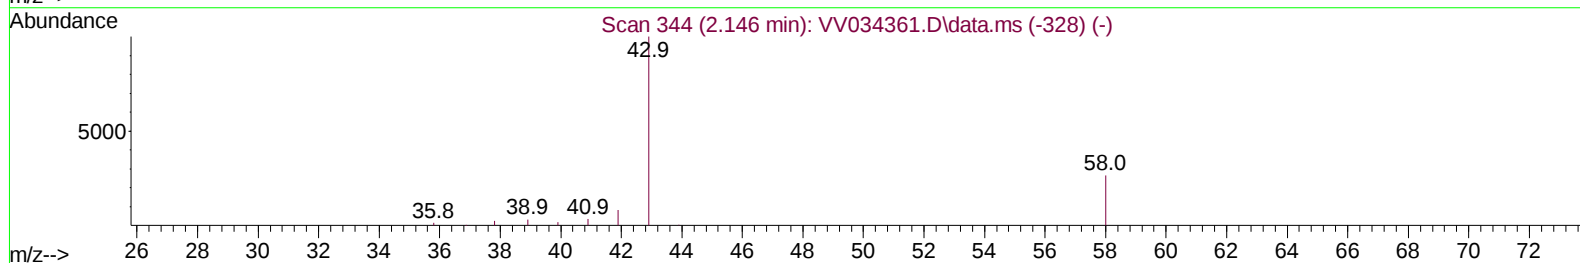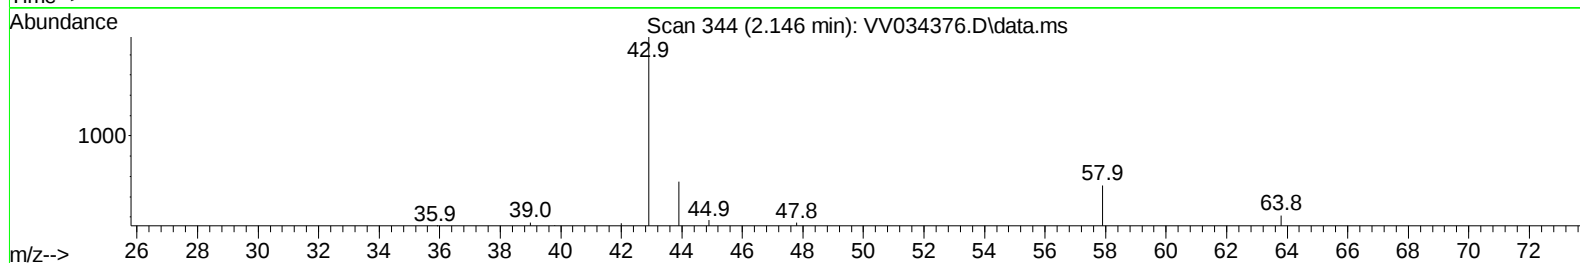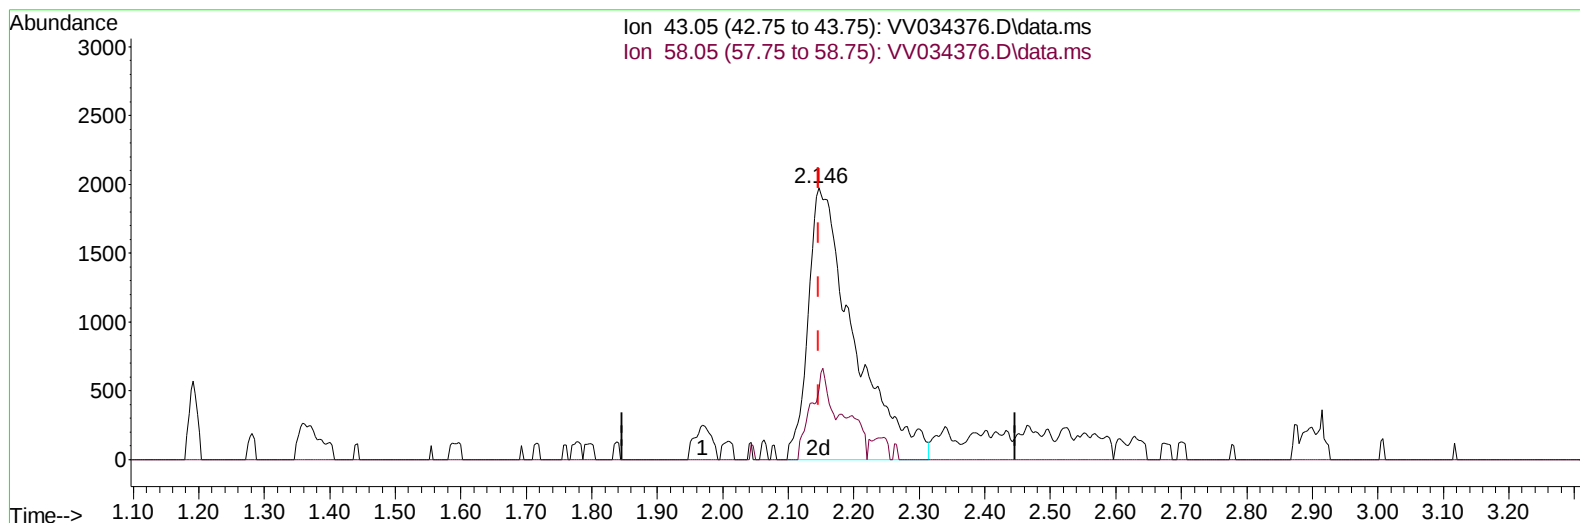

TIC: VV034376.D\data.ms

(13) Acetone (T)

2.146min (-0.000) 12.18 ug/L m

response 9566

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	6.90	0.43
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022324\
 Data File : VV034376.D
 Acq On : 23 Feb 2024 15:22
 Operator : SY/MD
 Sample : P1566-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JWAD2

Manual IntegrationsAPPROVED

Quant Time: Feb 24 00:48:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Feb 24 00:41:32 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/27/2024
 Supervised By :Semsettin Yesilyurt 02/27/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.538	114		79603	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117		71903	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152		34644	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		29319	4.756	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	95.200%	
7) Chloroethane-d5	1.535	69		24382	4.515	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	90.400%	
11) 1,1-Dichloroethene-d2	2.060	65		13595	4.573	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	91.400%	
20) 2-Butanone-d5	3.828	46		44291	42.777	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	85.560%	
24) Chloroform-d	4.249	84		51307	4.580	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	91.600%	
26) 1,2-Dichloroethane-d4	4.947	65		25383	4.848	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	97.000%	
32) Benzene-d6	4.963	84		98497	4.566	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	91.400%	
36) 1,2-Dichloropropane-d6	5.992	67		27204	4.511	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	90.200%	
41) Toluene-d8	7.246	98		89965	4.538	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	90.800%	
43) trans-1,3-Dichloroprop...	7.564	79		6088	2.674	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	53.400%#	
46) 2-Hexanone-d5	8.030	63		37094	45.635	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	91.260%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84		17760	4.858	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	97.200%	
66) 1,2-Dichlorobenzene-d4	11.561	152		30337	4.815	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	96.200%	
Target Compounds							
13) Acetone	2.146	43		9566m	12.178	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022324\
Data File : VV034376.D
Acq On : 23 Feb 2024 15:22
Operator : SY/MD
Sample : P1566-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
JWAD2

Manual IntegrationsAPPROVED

Quant Time: Feb 24 00:48:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Feb 24 00:41:32 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/27/2024
Supervised By :Semsettin Yesilyurt 02/27/2024

