

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022324\
 Data File : VW034366.D
 Acq On : 23 Feb 2024 11:20
 Operator : SY/MD
 Sample : P1566-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JWAC6

Quant Time: Feb 24 00:46:12 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Feb 24 00:41:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	66987	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	62910	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	30872	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	25167	4.851	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	97.000%	
7) Chloroethane-d5	1.532	69	20845	4.587	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	91.800%	
11) 1,1-Dichloroethene-d2	2.060	65	11686	4.671	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	93.400%	
20) 2-Butanone-d5	3.799	46	44994	51.640	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	103.280%	
24) Chloroform-d	4.253	84	43486	4.613	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.200%	
26) 1,2-Dichloroethane-d4	4.947	65	22757	5.166	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	103.400%	
32) Benzene-d6	4.960	84	81754	4.331	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.600%	
36) 1,2-Dichloropropane-d6	5.992	67	23809	4.513	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	90.200%	
41) Toluene-d8	7.246	98	74755	4.309	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	86.200%	
43) trans-1,3-Dichloroprop...	7.564	79	7526	3.778	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	75.600%	
46) 2-Hexanone-d5	8.027	63	35147	49.421	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	98.840%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84	16837	5.264	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	105.200%	
66) 1,2-Dichlorobenzene-d4	11.561	152	26069	4.643	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	92.800%	
Target Compounds					Qvalue	
13) Acetone	2.127	43	9522	14.405	ug/L #	36


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022324\
Data File : VV034366.D
Acq On : 23 Feb 2024 11:20
Operator : SY/MD
Sample : P1566-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JWAC6

Quant Time: Feb 24 00:46:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Feb 24 00:41:32 2024
Response via : Initial Calibration

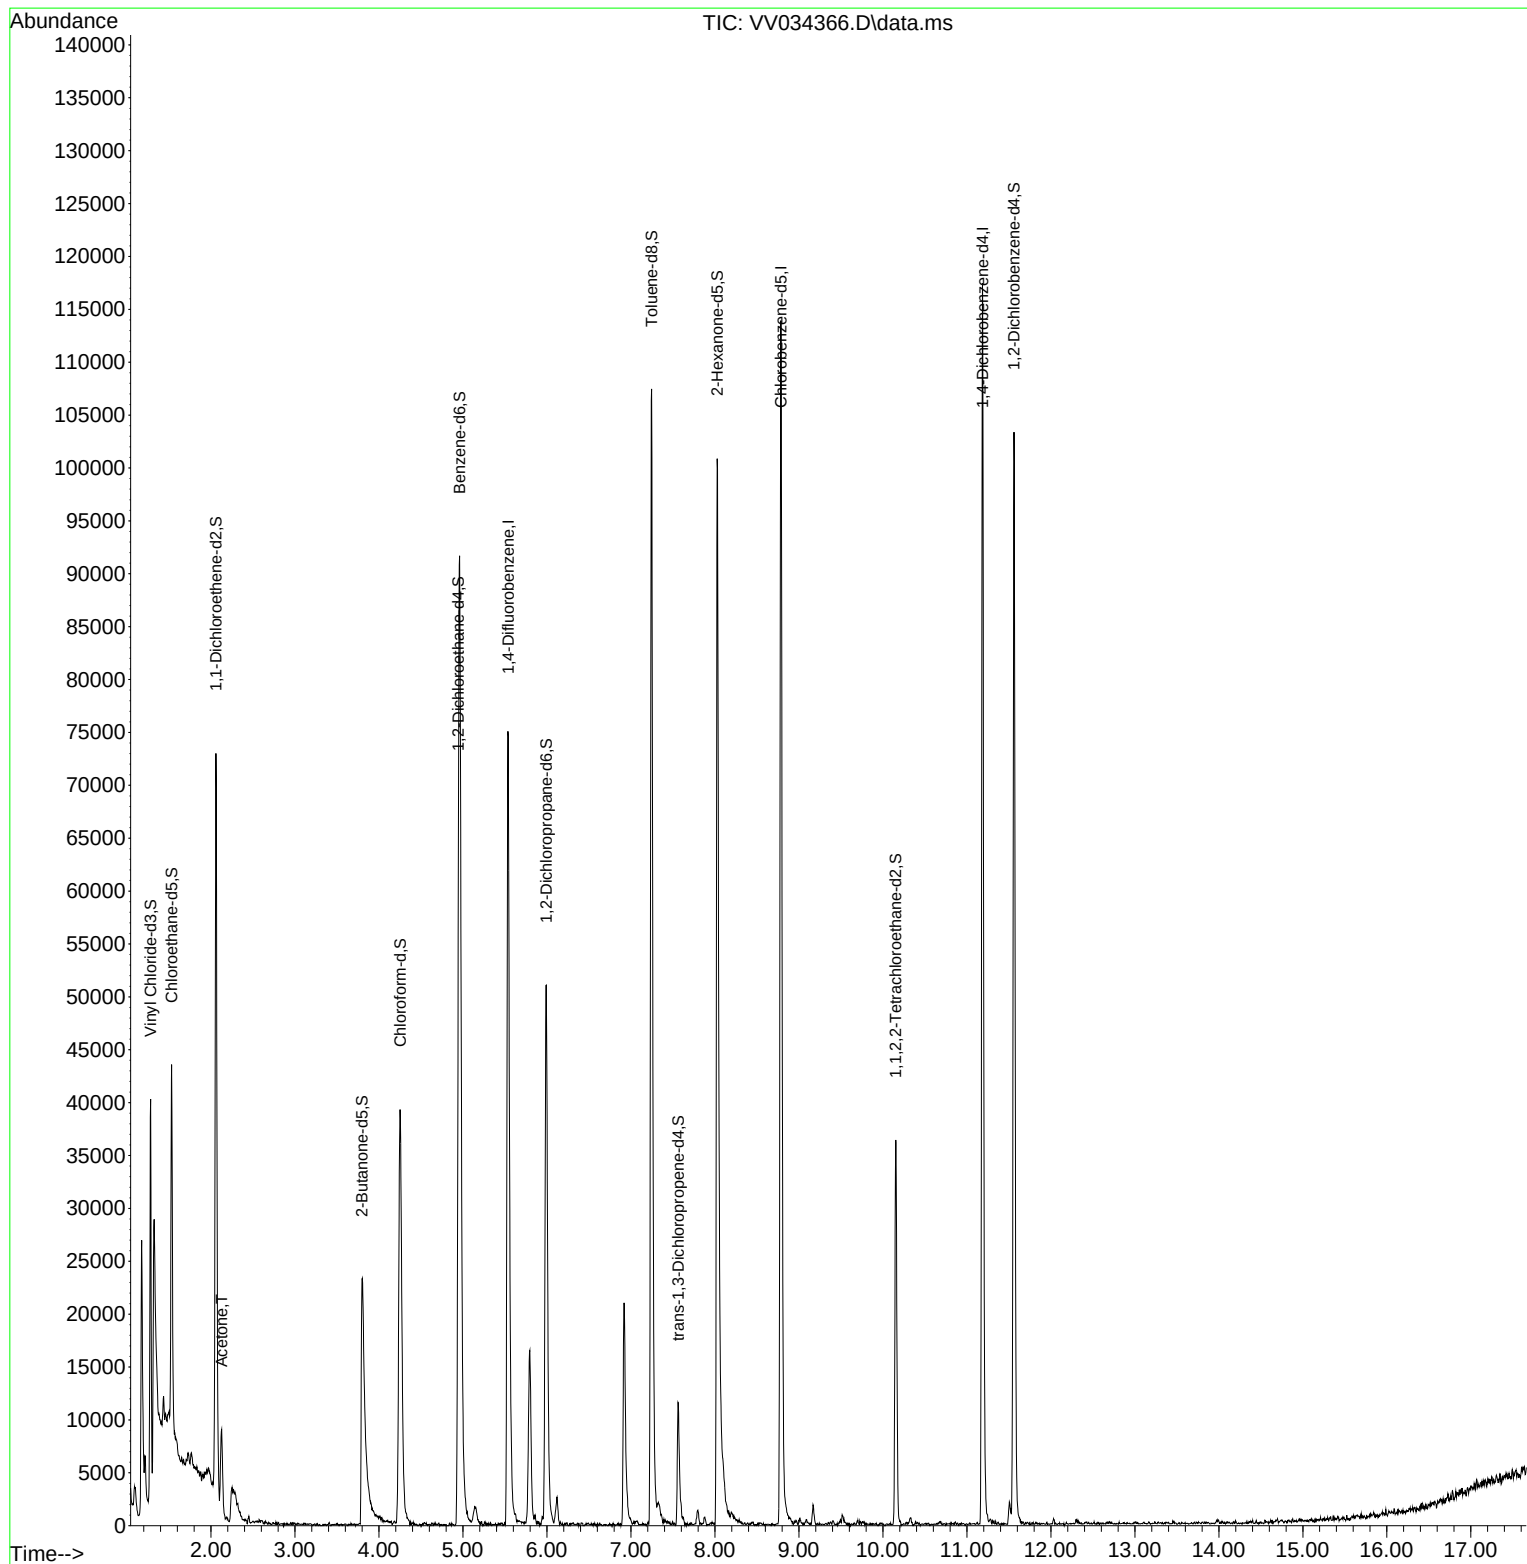

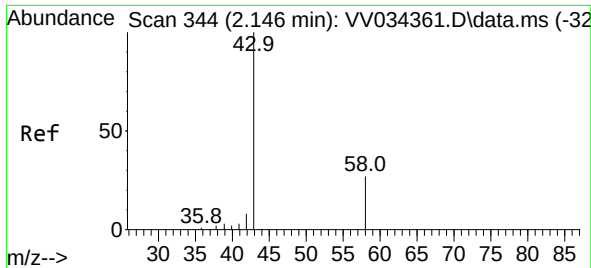

#13

Acetone

Concen: 14.405 ug/L

RT: 2.127 min Scan# 31

Delta R.T. -0.019 min

Lab File: VV034366.D

Acq: 23 Feb 2024 11:20

Instrument :

MSVOA_V

ClientSampleId :

JWAC6

Tgt Ion: 43 Resp: 9522

Ion Ratio Lower Upper

43 100

58 28.8 0.0 13.8#

