

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022324\
 Data File : VW034375.D
 Acq On : 23 Feb 2024 14:57
 Operator : SY/MD
 Sample : P1566-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JWAD0

Quant Time: Feb 24 00:48:30 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Feb 24 00:41:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	93531	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	88096	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	40441	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	29470	4.068	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.400%
7) Chloroethane-d5	1.532	69	24196	3.814	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.200%
11) 1,1-Dichloroethene-d2	2.060	65	13863	3.968	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.400%
20) 2-Butanone-d5	3.825	46	44792	36.818	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	73.640%
24) Chloroform-d	4.252	84	50315	3.823	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	76.400%
26) 1,2-Dichloroethane-d4	4.947	65	24903	4.048	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.000%
32) Benzene-d6	4.963	84	98837	3.739	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	74.800%
36) 1,2-Dichloropropane-d6	5.992	67	28345	3.836	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	76.800%
41) Toluene-d8	7.243	98	88674	3.650	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.000%
43) trans-1,3-Dichloroprop...	7.564	79	6283	2.252	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	45.000%#
46) 2-Hexanone-d5	8.030	63	36872	37.024	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	74.040%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	18008	4.020	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	80.400%
66) 1,2-Dichlorobenzene-d4	11.561	152	29782	4.049	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	81.000%
Target Compounds					Qvalue	
13) Acetone	2.146	43	18392	19.927	ug/L	# 71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022324\
Data File : VV034375.D
Acq On : 23 Feb 2024 14:57
Operator : SY/MD
Sample : P1566-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JWAD0

Quant Time: Feb 24 00:48:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Feb 24 00:41:32 2024
Response via : Initial Calibration

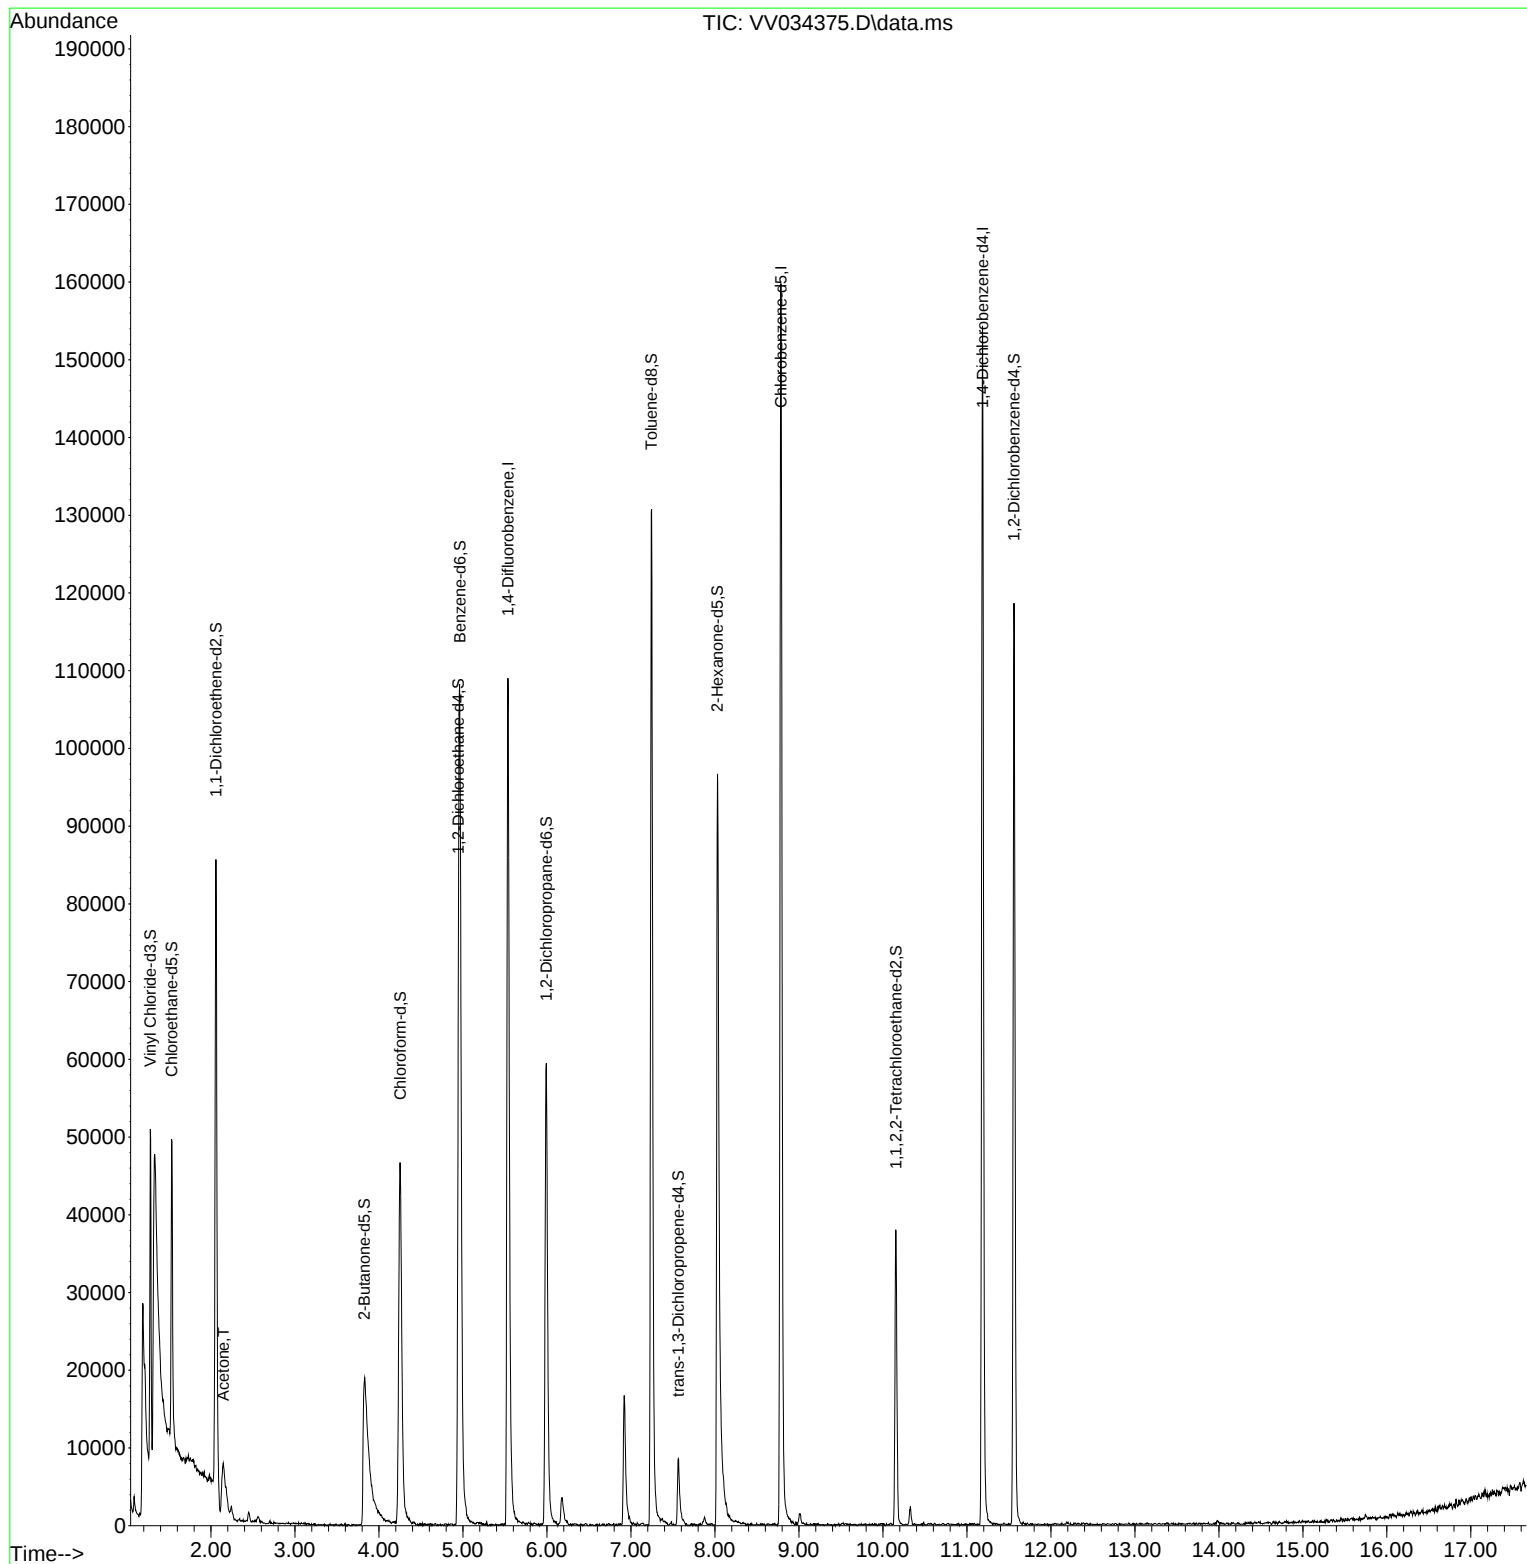

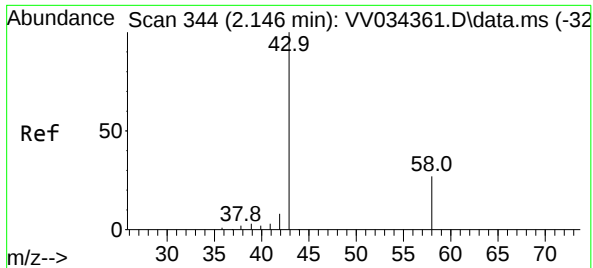

#13
 Acetone
 Concen: 19.927 ug/L
 RT: 2.146 min Scan# 34
 Delta R.T. -0.000 min
 Lab File: VV034375.D
 Acq: 23 Feb 2024 14:57

Instrument :
 MSVOA_V
 ClientSampleId :
 JWAD0

Tgt Ion: 43 Resp: 18392
 Ion Ratio Lower Upper
 43 100
 58 16.9 0.0 13.8#

