

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022324\
 Data File : VW034376.D
 Acq On : 23 Feb 2024 15:22
 Operator : SY/MD
 Sample : P1566-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JWAD2

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 02/27/2024
 Supervised By :Semsettin Yesilyurt 02/27/2024

Quant Time: Feb 24 00:48:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Feb 24 00:41:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	79603	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	71903	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	34644	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	29319	4.756	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	95.200%	
7) Chloroethane-d5	1.535	69	24382	4.515	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	90.400%	
11) 1,1-Dichloroethene-d2	2.060	65	13595	4.573	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	91.400%	
20) 2-Butanone-d5	3.828	46	44291	42.777	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	85.560%	
24) Chloroform-d	4.249	84	51307	4.580	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.600%	
26) 1,2-Dichloroethane-d4	4.947	65	25383	4.848	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.000%	
32) Benzene-d6	4.963	84	98497	4.566	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.400%	
36) 1,2-Dichloropropane-d6	5.992	67	27204	4.511	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	90.200%	
41) Toluene-d8	7.246	98	89965	4.538	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	90.800%	
43) trans-1,3-Dichloroprop...	7.564	79	6088	2.674	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	53.400%#	
46) 2-Hexanone-d5	8.030	63	37094	45.635	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	91.260%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	17760	4.858	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	97.200%	
66) 1,2-Dichlorobenzene-d4	11.561	152	30337	4.815	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.200%	
Target Compounds					Qvalue	
13) Acetone	2.146	43	9566m	12.178	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022324\
Data File : VV034376.D
Acq On : 23 Feb 2024 15:22
Operator : SY/MD
Sample : P1566-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
JWAD2

Quant Time: Feb 24 00:48:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Feb 24 00:41:32 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 02/27/2024
Supervised By :Semsettin Yesilyurt 02/27/2024

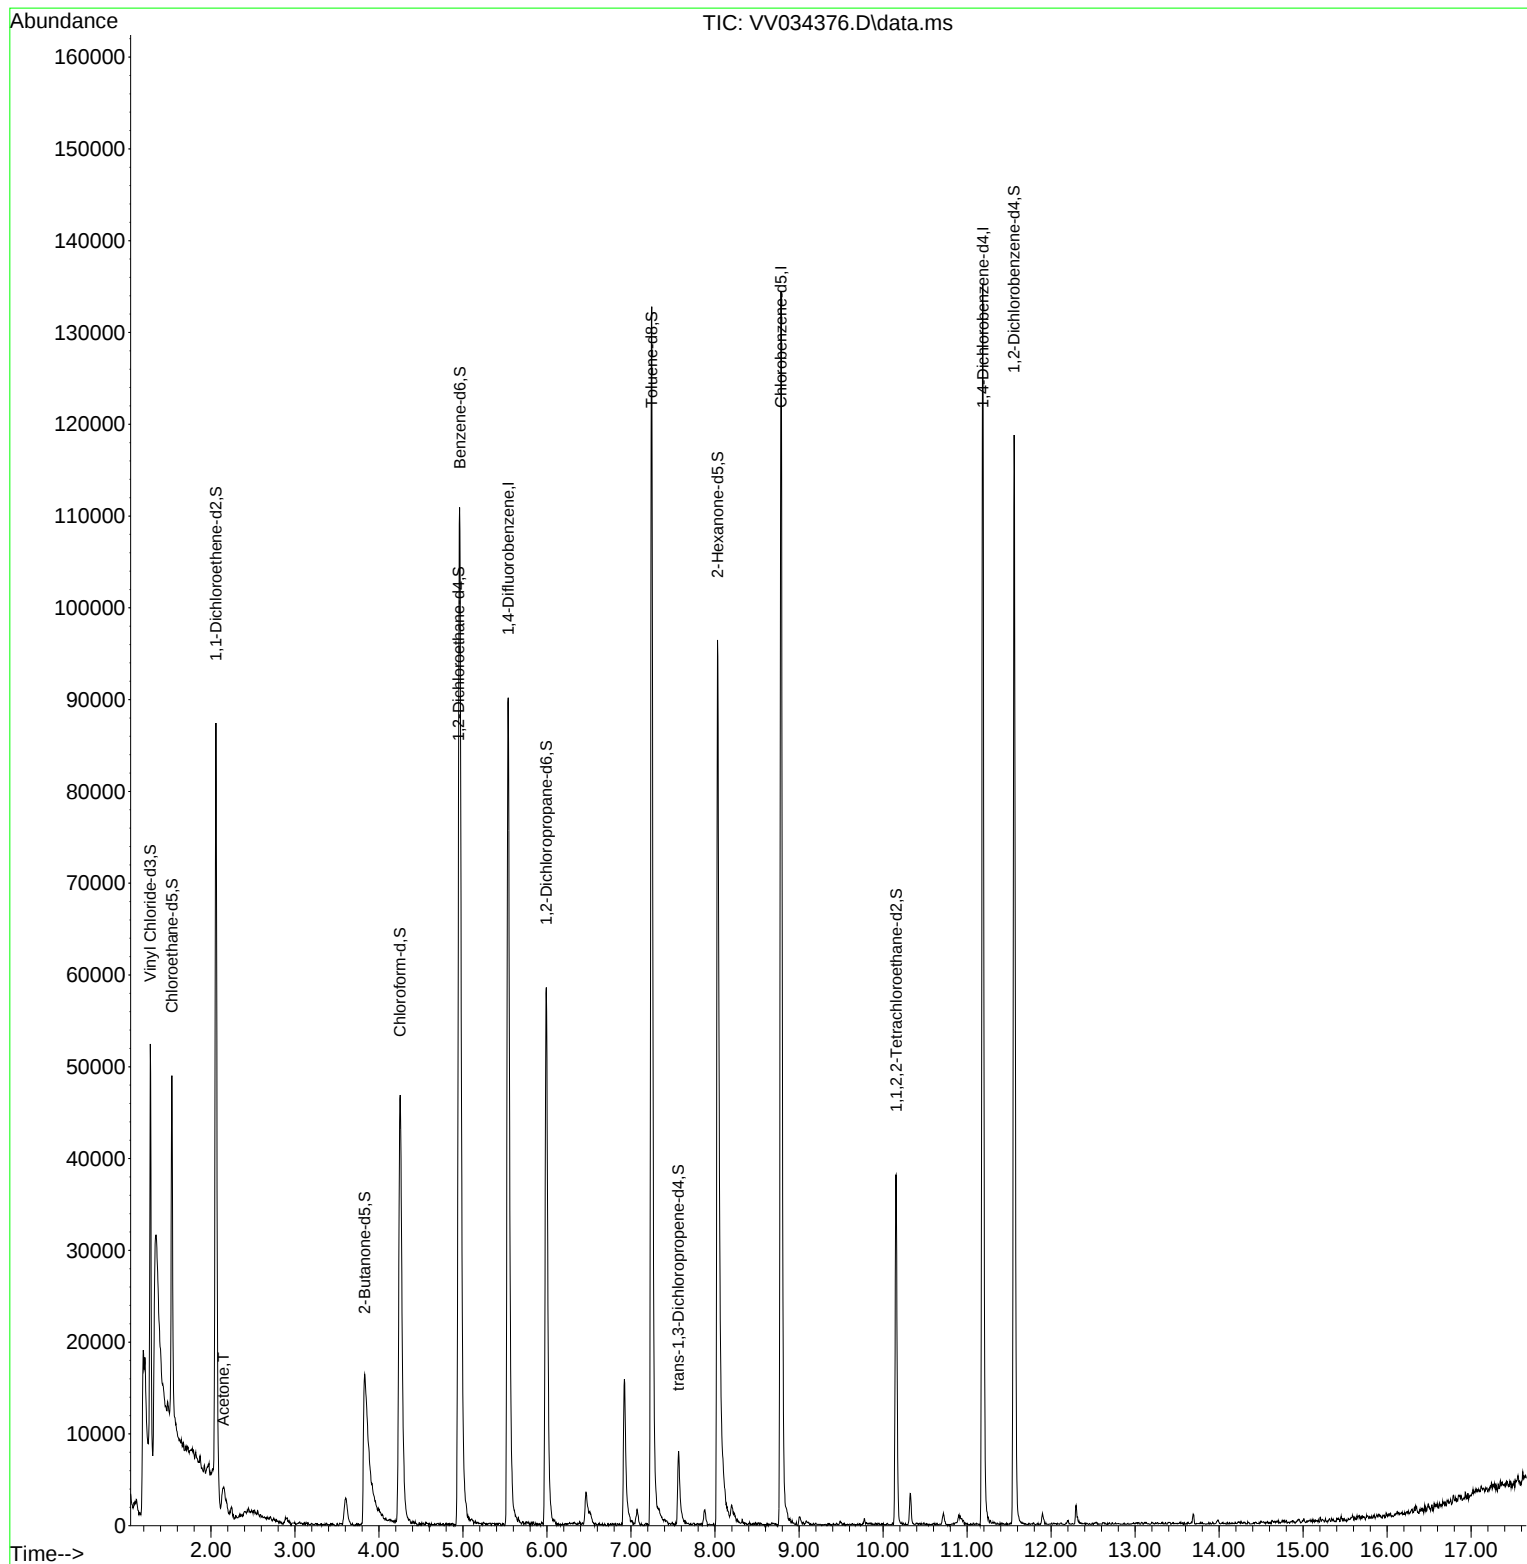

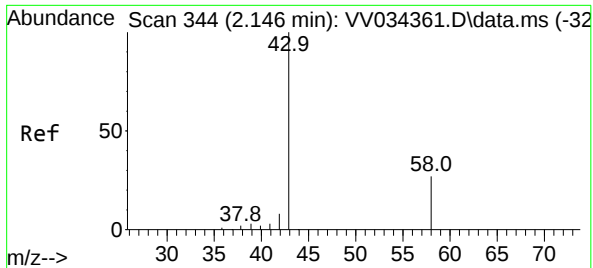

#13
 Acetone
 Concen: 12.178 ug/L m
 RT: 2.146 min Scan# 34
 Delta R.T. -0.000 min
 Lab File: VV034376.D
 Acq: 23 Feb 2024 15:22

Instrument :
 MSVOA_V
 ClientSampleId :
 JWAD2

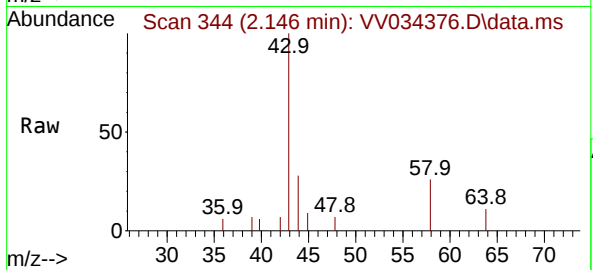

Tgt Ion: 43 Resp: 956
 Ion Ratio Lower Upper
 43 100
 58 0.4 0.0 13.8

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 02/27/2024
 Supervised By :Semsettin Yesilyurt 02/27/2024

