

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022324\
 Data File : VW034382.D
 Acq On : 23 Feb 2024 17:48
 Operator : SY/MD
 Sample : P1535-10 500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF7

Quant Time: Feb 24 00:50:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Feb 24 00:41:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	96606	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	91250	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	44493	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	31212	4.172	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	83.400%	
7) Chloroethane-d5	1.535	69	25606	3.907	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	78.200%	
11) 1,1-Dichloroethene-d2	2.059	65	14703	4.075	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	81.400%	
20) 2-Butanone-d5	3.812	46	52824	42.038	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	84.080%	
24) Chloroform-d	4.252	84	54871	4.036	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	80.800%	
26) 1,2-Dichloroethane-d4	4.947	65	27202	4.281	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.600%	
32) Benzene-d6	4.963	84	105467	3.852	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	77.000%	
36) 1,2-Dichloropropane-d6	5.992	67	30366	3.968	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	79.400%	
41) Toluene-d8	7.246	98	94091	3.740	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	74.800%	
43) trans-1,3-Dichloroprop...	7.564	79	6765	2.341	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	46.800%#	
46) 2-Hexanone-d5	8.027	63	42846	41.535	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	83.080%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	18914	4.077	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	81.600%	
66) 1,2-Dichlorobenzene-d4	11.561	152	34075	4.211	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	84.200%	
Target Compounds						Qvalue
16) Methylene chloride	2.449	84	1255	0.194	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022324\
Data File : VV034382.D
Acq On : 23 Feb 2024 17:48
Operator : SY/MD
Sample : P1535-10 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF7


Quant Time: Feb 24 00:50:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Feb 24 00:41:32 2024
Response via : Initial Calibration

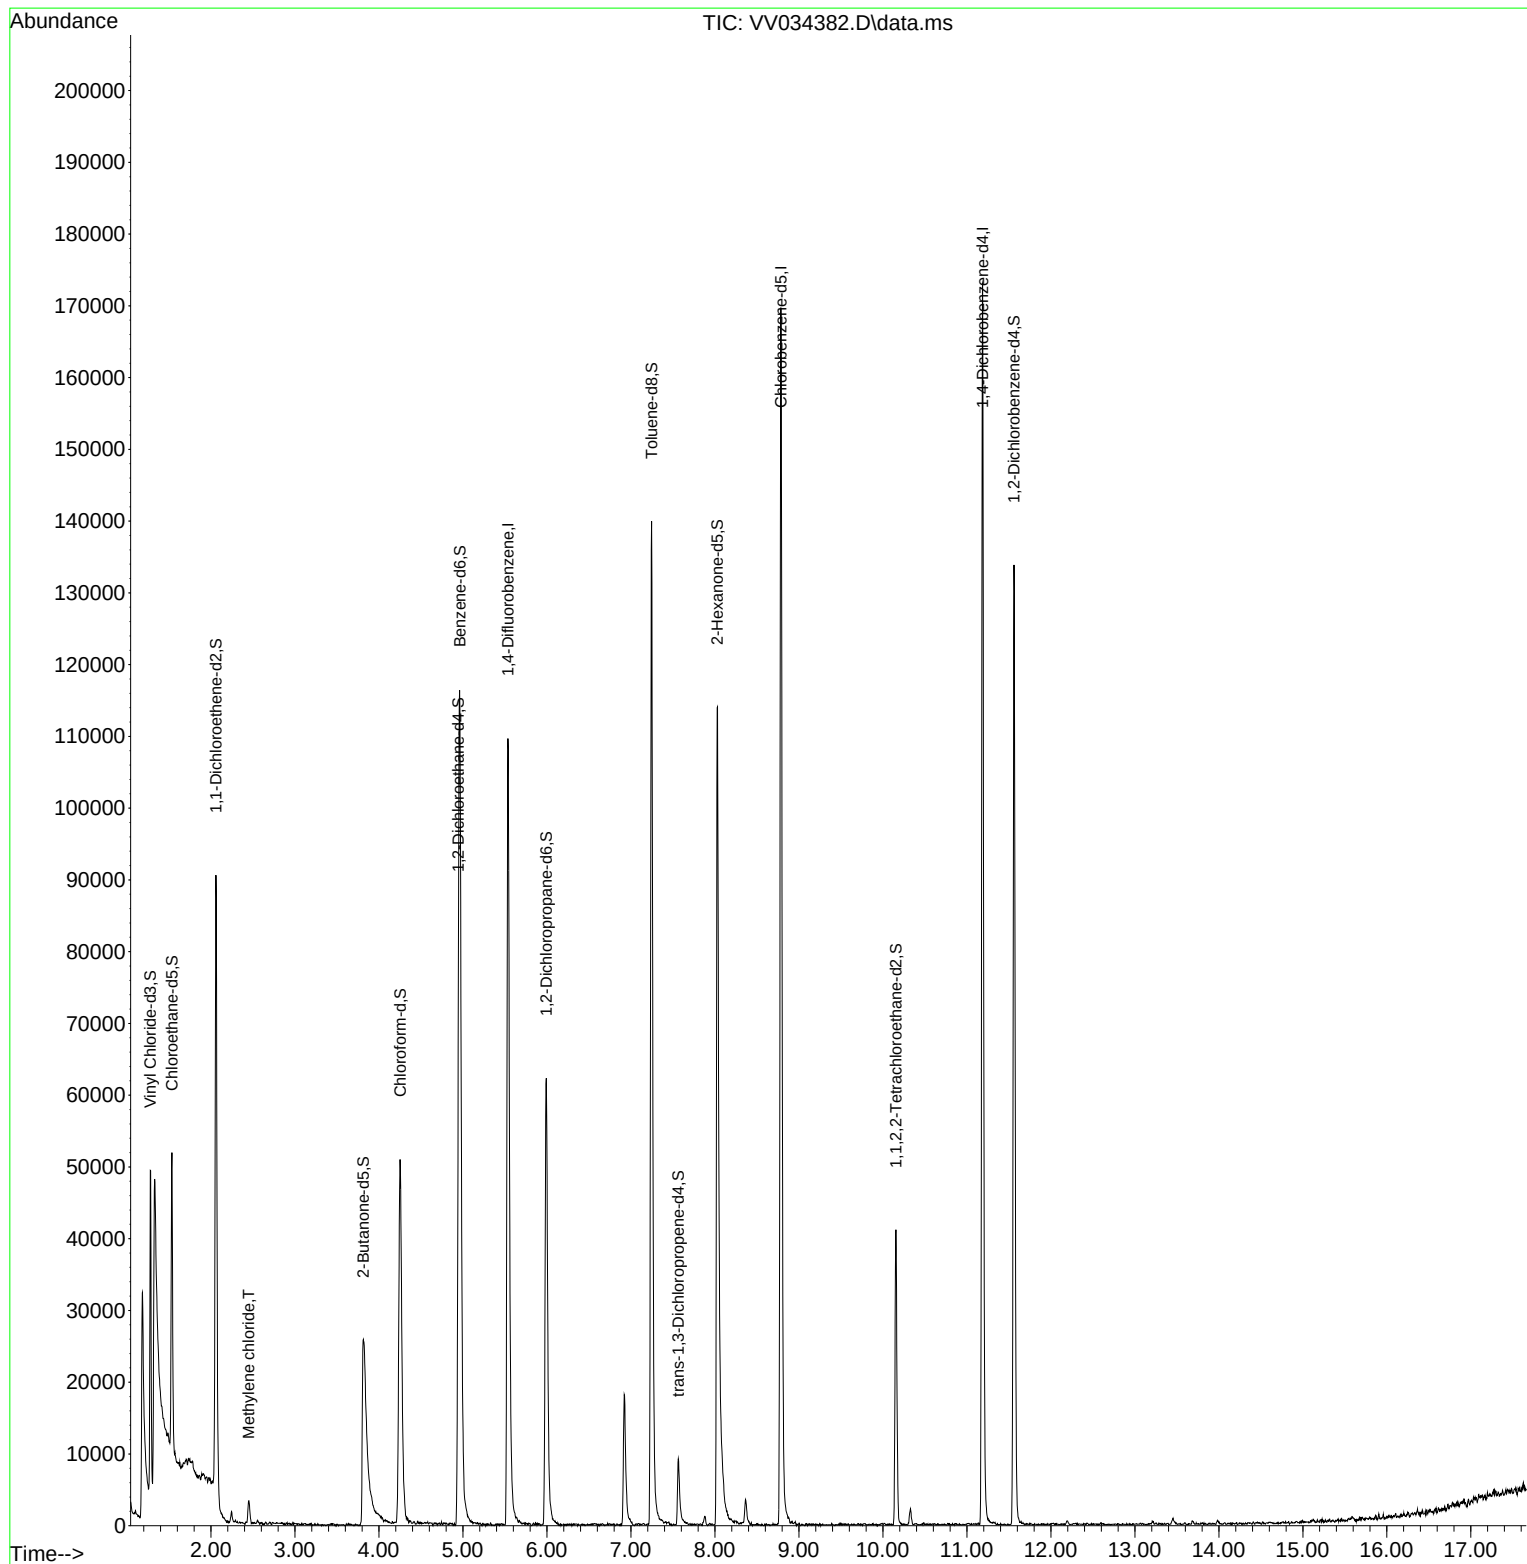

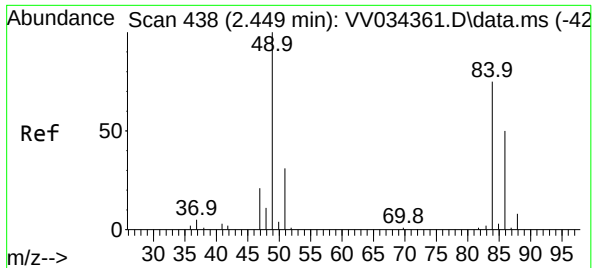

#16
Methylene chloride
Concen: 0.194 ug/L
RT: 2.449 min Scan# 41
Delta R.T. -0.000 min
Lab File: VV034382.D
Acq: 23 Feb 2024 17:48

Instrument :
MSVOA_V
ClientSampleId :
C0AF7

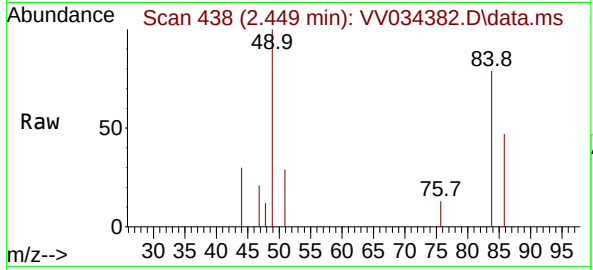

Tgt Ion:	84	Resp:	1255
Ion	Ratio	Lower	Upper
84	100		
86	60.0	44.7	83.1
49	126.4	93.7	173.9

