

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV022324\  
 Data File : VV034367.D  
 Acq On : 23 Feb 2024 11:44  
 Operator : SY/MD  
 Sample : VIBLK326  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 VIBLK326

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR012524WMA.M  
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV034367.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.172       | 35            | 41          | 51           | rBV      | 27464          | 32314         | 4.90%           | 1.374%        |
| 2         | 1.294       | 62            | 79          | 102          | rBV      | 251674         | 659678        | 100.00%         | 28.042%       |
| 3         | 2.060       | 309           | 317         | 330          | rVB3     | 41627          | 69400         | 10.52%          | 2.950%        |
| 4         | 2.243       | 364           | 374         | 386          | rBV      | 15985          | 29090         | 4.41%           | 1.237%        |
| 5         | 2.452       | 428           | 439         | 456          | rBV2     | 7873           | 13400         | 2.03%           | 0.570%        |
| 6         | 2.561       | 461           | 473         | 495          | rVV2     | 6888           | 17846         | 2.71%           | 0.759%        |
| 7         | 2.696       | 504           | 515         | 542          | rBV2     | 284263         | 543791        | 82.43%          | 23.116%       |
| 8         | 3.114       | 633           | 645         | 661          | rVB3     | 3031           | 6709          | 1.02%           | 0.285%        |
| 9         | 3.812       | 846           | 862         | 898          | rBV4     | 53651          | 171677        | 26.02%          | 7.298%        |
| 10        | 4.256       | 985           | 1000        | 1028         | rVB2     | 17283          | 44980         | 6.82%           | 1.912%        |
| 11        | 4.963       | 1206          | 1220        | 1249         | rBV3     | 40361          | 106774        | 16.19%          | 4.539%        |
| 12        | 5.542       | 1390          | 1400        | 1425         | rBV2     | 30421          | 62971         | 9.55%           | 2.677%        |
| 13        | 5.995       | 1529          | 1541        | 1565         | rBV2     | 21917          | 45315         | 6.87%           | 1.926%        |
| 14        | 6.924       | 1822          | 1830        | 1846         | rBV2     | 8252           | 16906         | 2.56%           | 0.719%        |
| 15        | 7.249       | 1921          | 1931        | 1951         | rBV      | 44678          | 81952         | 12.42%          | 3.484%        |
| 16        | 7.567       | 2021          | 2030        | 2047         | rBV3     | 4738           | 9437          | 1.43%           | 0.401%        |
| 17        | 8.027       | 2164          | 2173        | 2202         | rBV      | 85229          | 165587        | 25.10%          | 7.039%        |
| 18        | 8.789       | 2401          | 2410        | 2431         | rBV      | 46133          | 78713         | 11.93%          | 3.346%        |
| 19        | 10.156      | 2825          | 2835        | 2847         | rBV2     | 25418          | 39574         | 6.00%           | 1.682%        |
| 20        | 11.188      | 3146          | 3156        | 3177         | rBV2     | 47264          | 75816         | 11.49%          | 3.223%        |
| 21        | 11.564      | 3263          | 3273        | 3296         | rVB      | 47944          | 80544         | 12.21%          | 3.424%        |




Sum of corrected areas: 2352474

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV022324\  
Data File : VV034367.D  
Acq On : 23 Feb 2024 11:44  
Operator : SY/MD  
Sample : VIBLK326  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
VIBLK326

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR012524WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

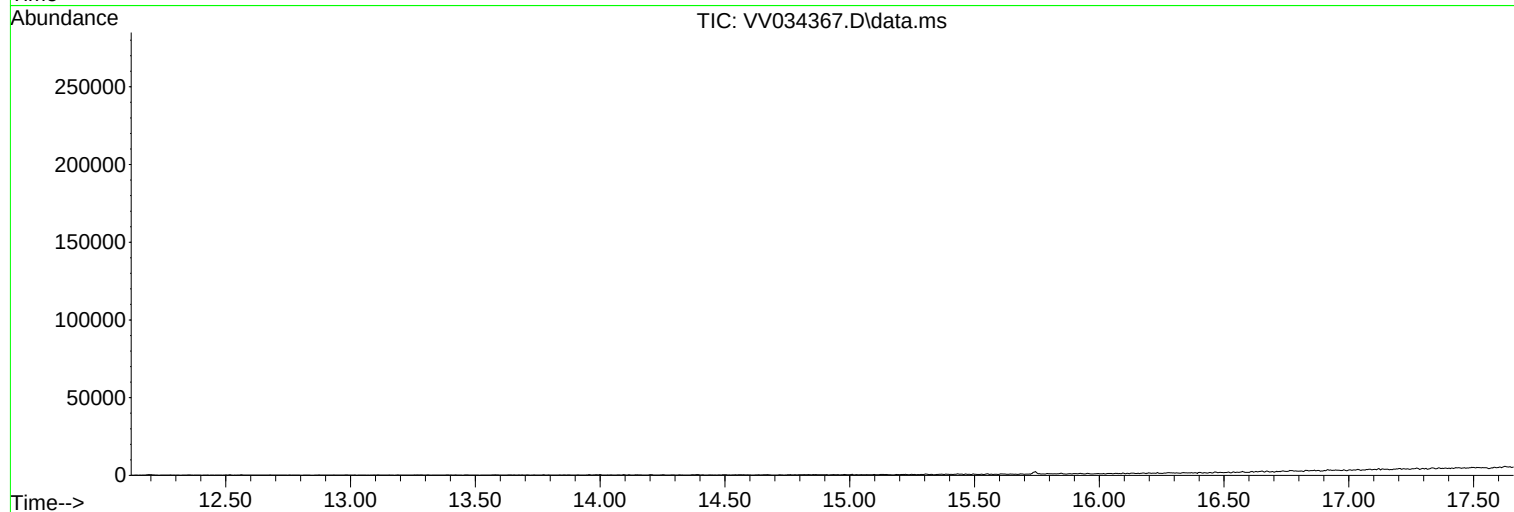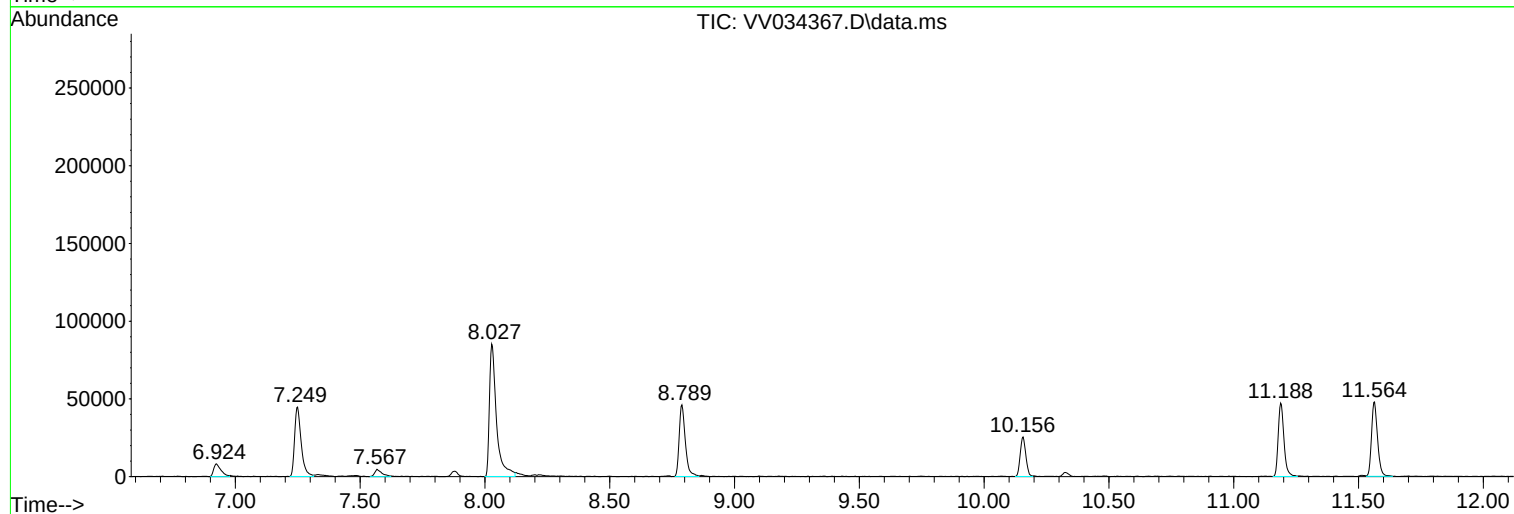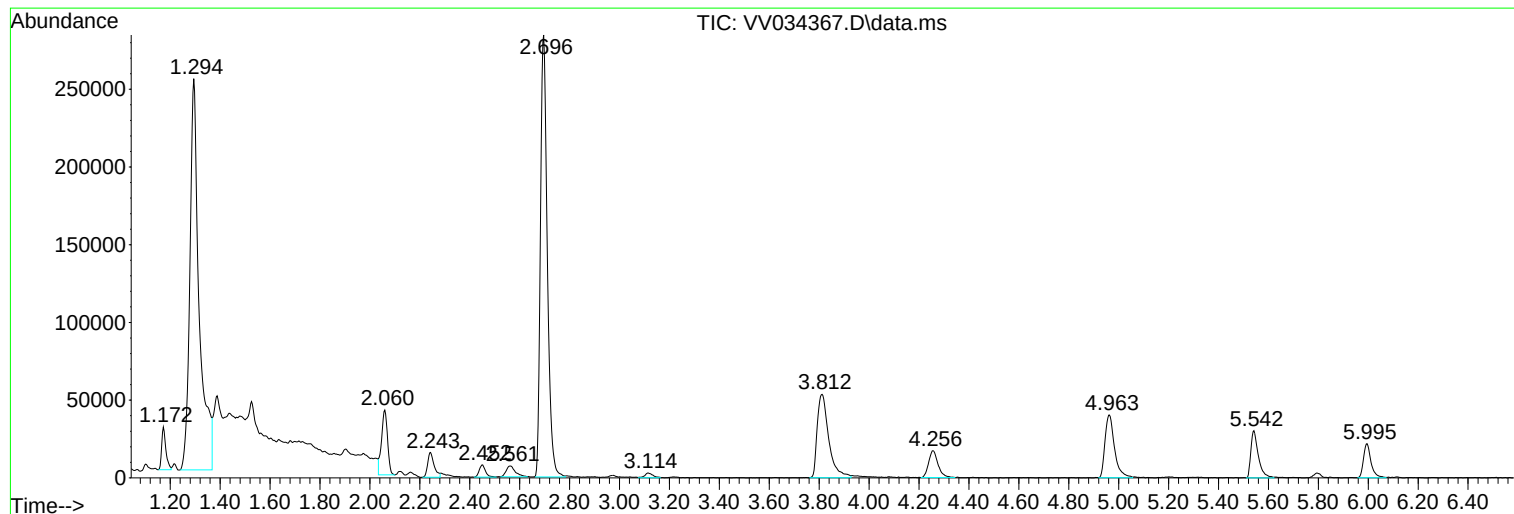

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV022324\  
Data File : VV034367.D  
Acq On : 23 Feb 2024 11:44  
Operator : SY/MD  
Sample : VIBLK326  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
VIBLK326

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR012524WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV022324\  
Data File : VV034367.D  
Acq On : 23 Feb 2024 11:44  
Operator : SY/MD  
Sample : VIBLK326  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
VIBLK326

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR012524WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |