

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022324\
 Data File : VV034368.D
 Acq On : 23 Feb 2024 12:09
 Operator : SY/MD
 Sample : VIBLK327
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK327

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034368.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	35	41	51	rBV	68914	89078	12.43%	3.434%
2	1.301	65	81	108	rBV2	193867	542067	75.67%	20.898%
3	1.529	149	152	182	rVB3	27220	54094	7.55%	2.085%
4	2.060	309	317	332	rVB2	43726	78216	10.92%	3.015%
5	2.240	363	373	387	rBV	16772	27209	3.80%	1.049%
6	2.696	503	515	542	rBV2	370876	716379	100.00%	27.618%
7	3.117	634	646	657	rBV4	3765	8040	1.12%	0.310%
8	3.812	849	862	891	rBV5	52105	150926	21.07%	5.819%
9	4.256	985	1000	1022	rBV2	19595	50671	7.07%	1.953%
10	4.960	1204	1219	1249	rBV3	48878	128189	17.89%	4.942%
11	5.542	1389	1400	1422	rBV2	35349	74098	10.34%	2.857%
12	5.992	1529	1540	1563	rBV2	25516	53392	7.45%	2.058%
13	6.921	1821	1829	1848	rBV3	9834	19645	2.74%	0.757%
14	7.246	1921	1930	1950	rBV	53071	95790	13.37%	3.693%
15	7.571	2022	2031	2050	rBV3	5108	11386	1.59%	0.439%
16	8.027	2165	2173	2201	rBV	91387	175955	24.56%	6.783%
17	8.789	2400	2410	2431	rBV	54673	92882	12.97%	3.581%
18	10.156	2823	2835	2850	rBV	28845	44925	6.27%	1.732%
19	11.188	3147	3156	3181	rBV	55265	87717	12.24%	3.382%
20	11.564	3262	3273	3292	rBV	56403	93234	13.01%	3.594%




Sum of corrected areas: 2593893

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022324\
Data File : VV034368.D
Acq On : 23 Feb 2024 12:09
Operator : SY/MD
Sample : VIBLK327
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK327

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

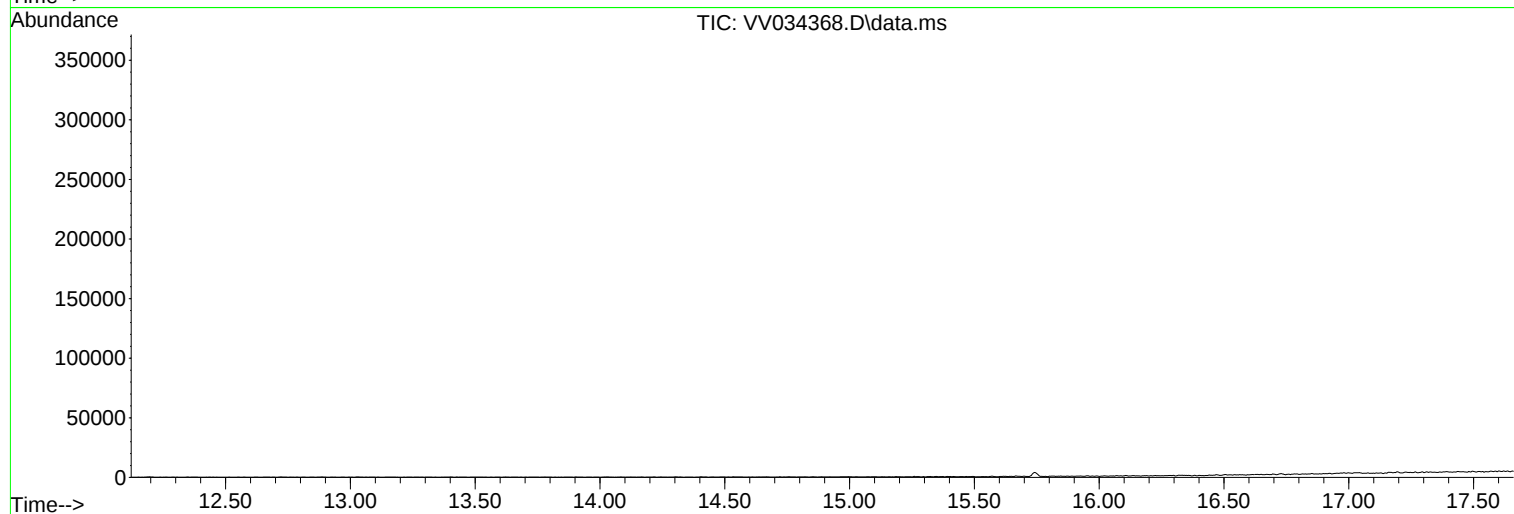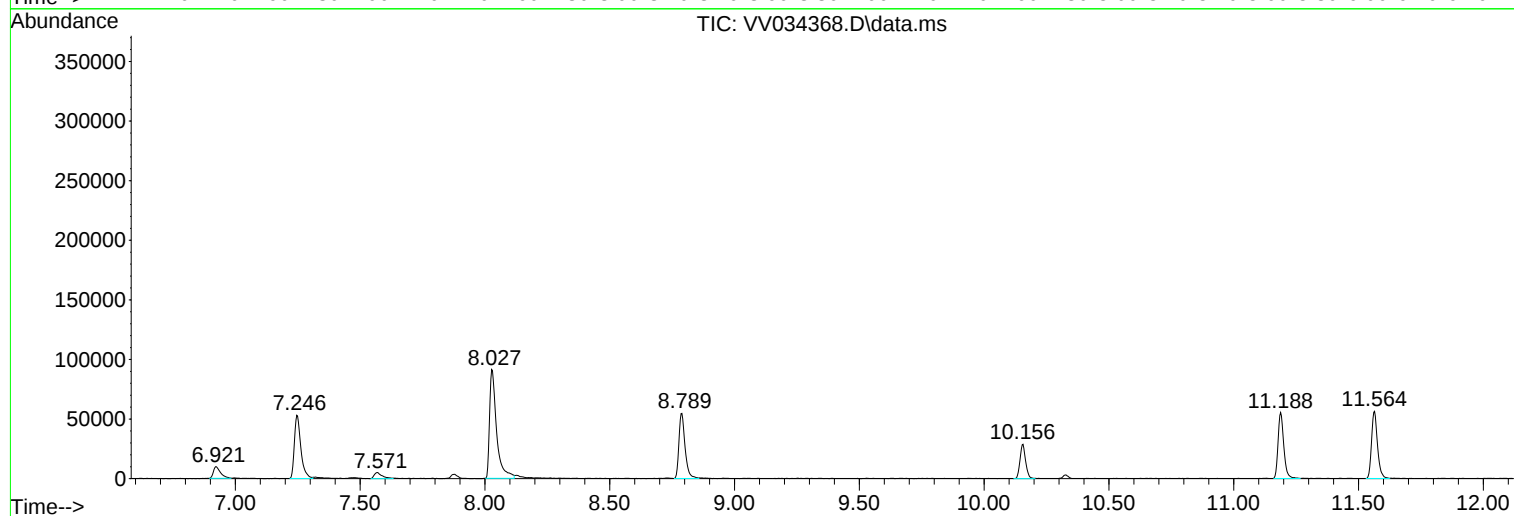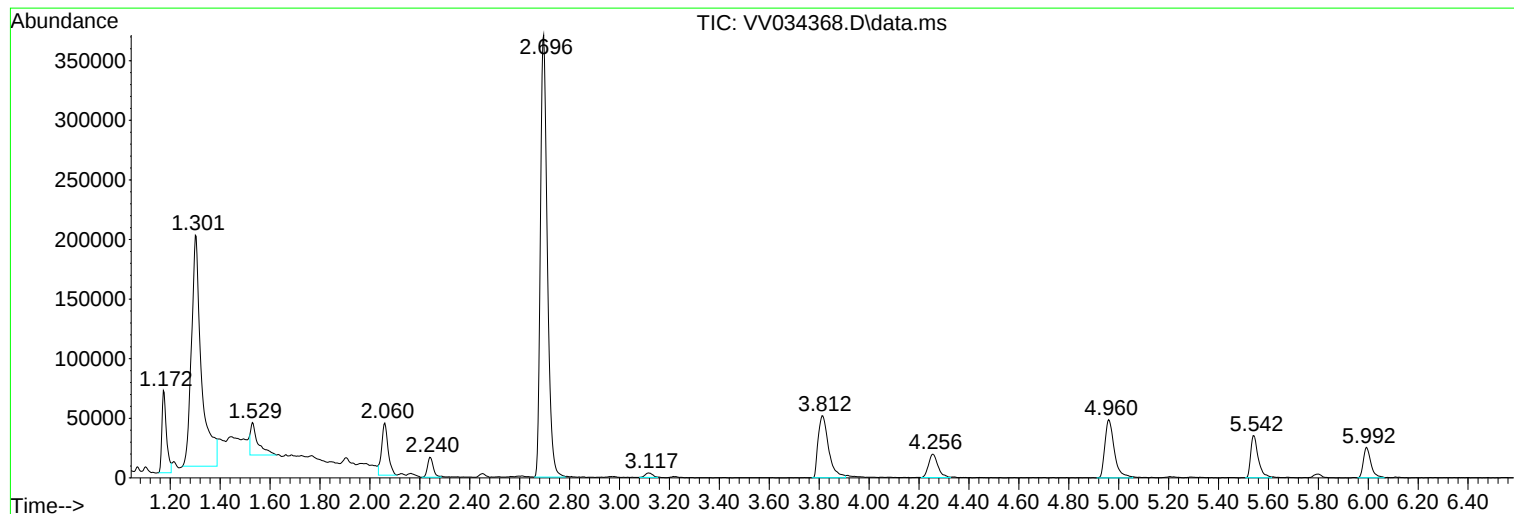

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022324\
Data File : VV034368.D
Acq On : 23 Feb 2024 12:09
Operator : SY/MD
Sample : VIBLK327
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK327

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022324\
Data File : VV034368.D
Acq On : 23 Feb 2024 12:09
Operator : SY/MD
Sample : VIBLK327
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK327

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc