


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022324\
Data File : VV034360.D
Acq On : 23 Feb 2024 08:18
Operator : SY/MD
Sample : BFB259
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB259

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Feb 24 00:41:32 2024

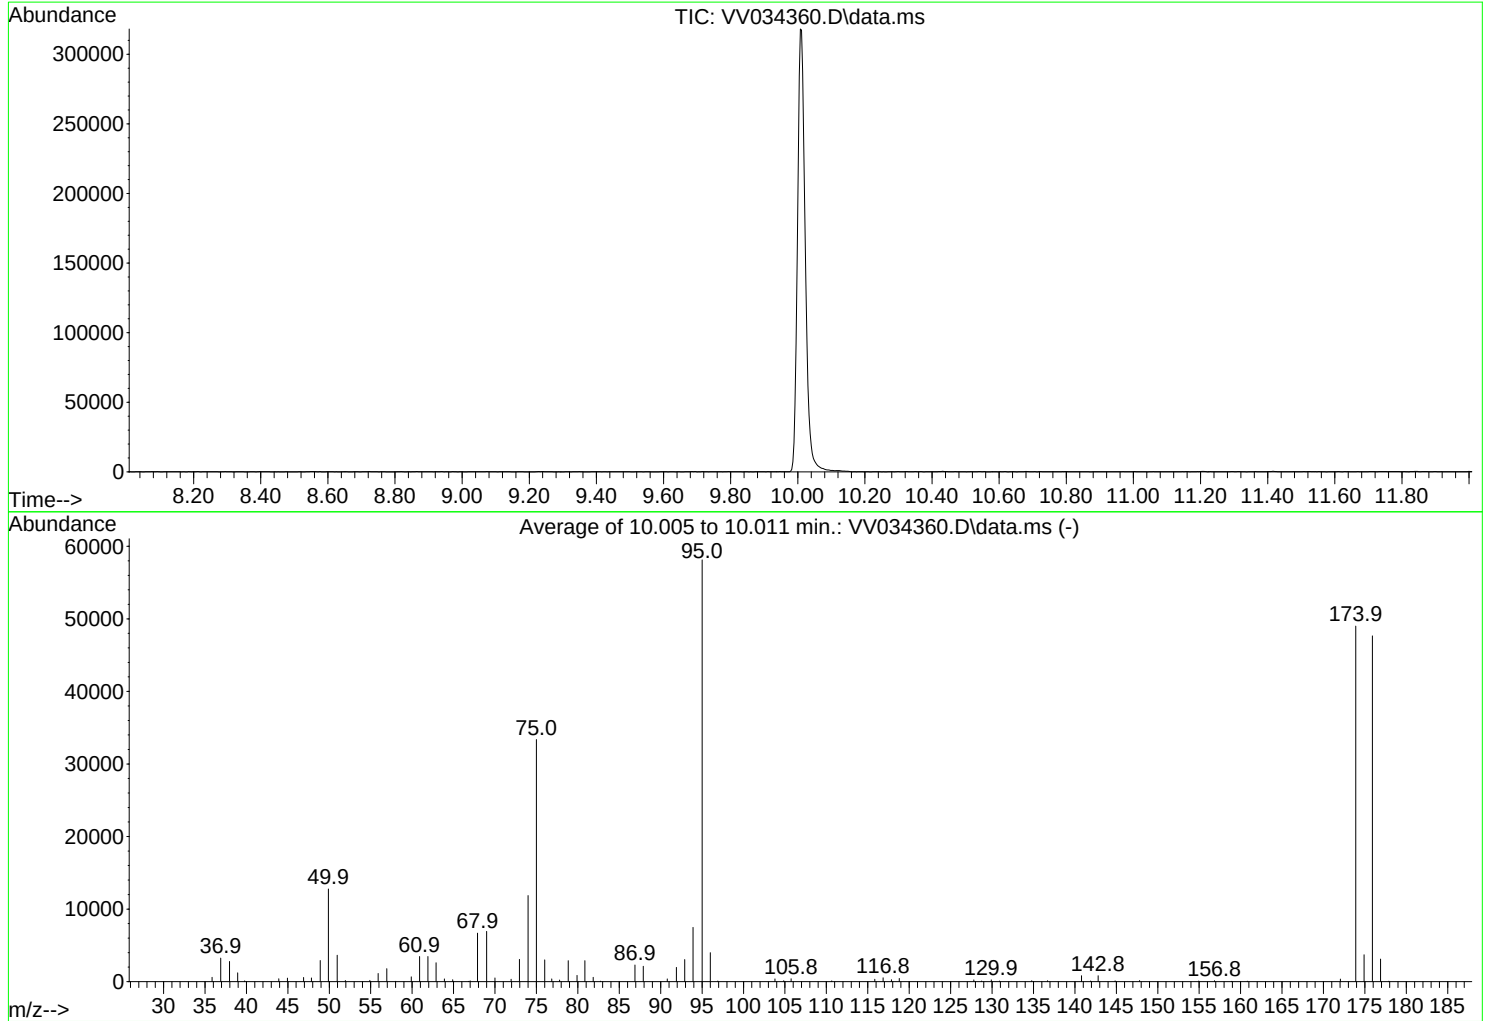

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	12766	PASS
75	95	30	80	57.4	33357	PASS
95	95	100	100	100.0	58133	PASS
96	95	5	9	6.9	4003	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.3	48995	PASS
175	174	5	9	7.6	3704	PASS
176	174	95	105	97.3	47656	PASS
177	176	5	10	6.5	3109	PASS

m/z	Abundance
44.00	150.0

Instrument :
MSVOA_V
ClientSampleId :
BFB259

m/z	Abundance
35.80	547.0
36.90	2909.0
38.00	2722.0
39.00	1163.0
39.80	114.0
43.90	518.0
44.90	498.0
46.90	492.0
47.80	520.0
48.90	2801.0
49.90	12012.0
51.00	3456.0
51.90	138.0
54.90	140.0
55.90	1031.0
57.00	1543.0
59.90	653.0
60.90	3276.0
61.90	3291.0
62.90	2516.0
63.90	381.0
64.90	298.0
66.80	140.0
67.90	6482.0
69.00	6446.0
70.00	440.0
71.90	344.0
73.00	2894.0
74.00	11058.0
75.00	31096.0
76.00	2828.0
76.80	342.0
77.80	200.0
78.80	2727.0
79.90	803.0
80.90	2766.0
81.90	591.0
82.70	110.0
86.90	2154.0
87.90	2002.0
90.80	383.0
91.90	1818.0
92.90	2960.0
93.90	6970.0
95.00	54224.0
96.00	3728.0
103.80	335.0
104.90	119.0
105.70	374.0
110.70	111.0
115.80	274.0
116.90	499.0
117.90	253.0
118.80	443.0
127.80	224.0
129.90	208.0
134.80	115.0
136.70	135.0
140.80	769.0
142.80	723.0
144.90	127.0
147.80	158.0
156.80	122.0
158.90	108.0
160.80	105.0
172.10	359.0
173.90	44416.0
174.90	3516.0
175.90	43368.0
176.90	2898.0

Instrument :
MSVOA_V
ClientSampleId :
BFB259

m/z	Abundance
35.90	628.0
36.90	3389.0
38.00	2877.0
39.00	1234.0
39.80	129.0
43.90	562.0
45.00	522.0
46.90	590.0
47.80	545.0
48.90	3027.0
49.90	13253.0
50.90	3755.0
51.90	156.0
54.90	179.0
55.90	1168.0
57.00	1845.0
58.00	104.0
59.90	688.0
60.90	3590.0
61.90	3601.0
62.90	2671.0
63.90	393.0
64.90	281.0
67.00	161.0
67.90	6919.0
69.00	7147.0
70.00	532.0
71.90	333.0
73.00	3150.0
74.00	12332.0
75.00	34624.0
76.00	3081.0
76.90	385.0
77.80	224.0
78.90	2999.0
79.90	902.0
80.90	2989.0
81.80	598.0
82.80	103.0
86.90	2379.0
87.90	2184.0
90.80	409.0
91.90	2047.0
92.90	3115.0
93.90	7713.0
95.00	60416.0
96.00	4186.0
96.90	133.0
103.80	395.0
104.80	129.0
105.80	400.0
110.70	121.0
115.90	373.0
116.90	566.0
117.90	269.0
118.80	461.0
127.80	242.0
128.80	107.0
129.90	267.0
130.90	117.0
134.80	134.0
136.70	150.0
140.80	837.0
141.90	113.0
142.80	818.0
144.90	126.0
147.80	166.0
155.00	126.0
156.80	140.0
160.80	109.0
172.00	347.0
173.90	50816.0
174.90	3838.0
175.90	49376.0
176.90	3197.0
177.90	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB259

m/z	Abundance
35.90	607.0
36.90	3435.0
37.90	2717.0
38.90	1218.0
39.80	116.0
43.90	540.0
45.00	470.0
46.90	660.0
47.90	473.0
48.90	2942.0
49.90	13032.0
50.90	3738.0
52.00	165.0
54.90	214.0
55.90	1188.0
56.90	1989.0
59.90	652.0
60.90	3520.0
61.90	3488.0
62.90	2600.0
63.90	334.0
64.90	253.0
67.00	174.0
67.90	6640.0
69.00	7188.0
70.00	543.0
72.00	335.0
72.90	3155.0
74.00	12220.0
75.00	34352.0
76.00	3070.0
76.90	401.0
77.80	229.0
78.90	2929.0
79.90	850.0
80.80	2932.0
81.80	605.0
86.90	2319.0
87.90	2149.0
90.80	347.0
91.90	2053.0
92.90	3064.0
93.90	7773.0
95.00	59760.0
96.00	4096.0
96.90	152.0
103.80	389.0
104.80	118.0
105.80	436.0
110.60	113.0
115.80	380.0
116.80	536.0
117.80	265.0
118.80	427.0
127.80	277.0
128.70	126.0
129.90	282.0
130.90	120.0
134.80	151.0
136.70	142.0
140.80	818.0
141.90	134.0
142.80	888.0
144.80	109.0
147.80	170.0
154.90	156.0
156.90	141.0
172.00	347.0
173.90	51752.0
174.90	3759.0
175.90	50224.0
176.90	3233.0
177.90	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB259