


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV022420\
 Data File : VV014689.D
 Acq On : 24 Feb 2020 09:49
 Operator : SY/MD
 Sample : BFB95
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB95

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
 Title : VOC Analysis
 Last Update : Tue Feb 25 06:37:27 2020

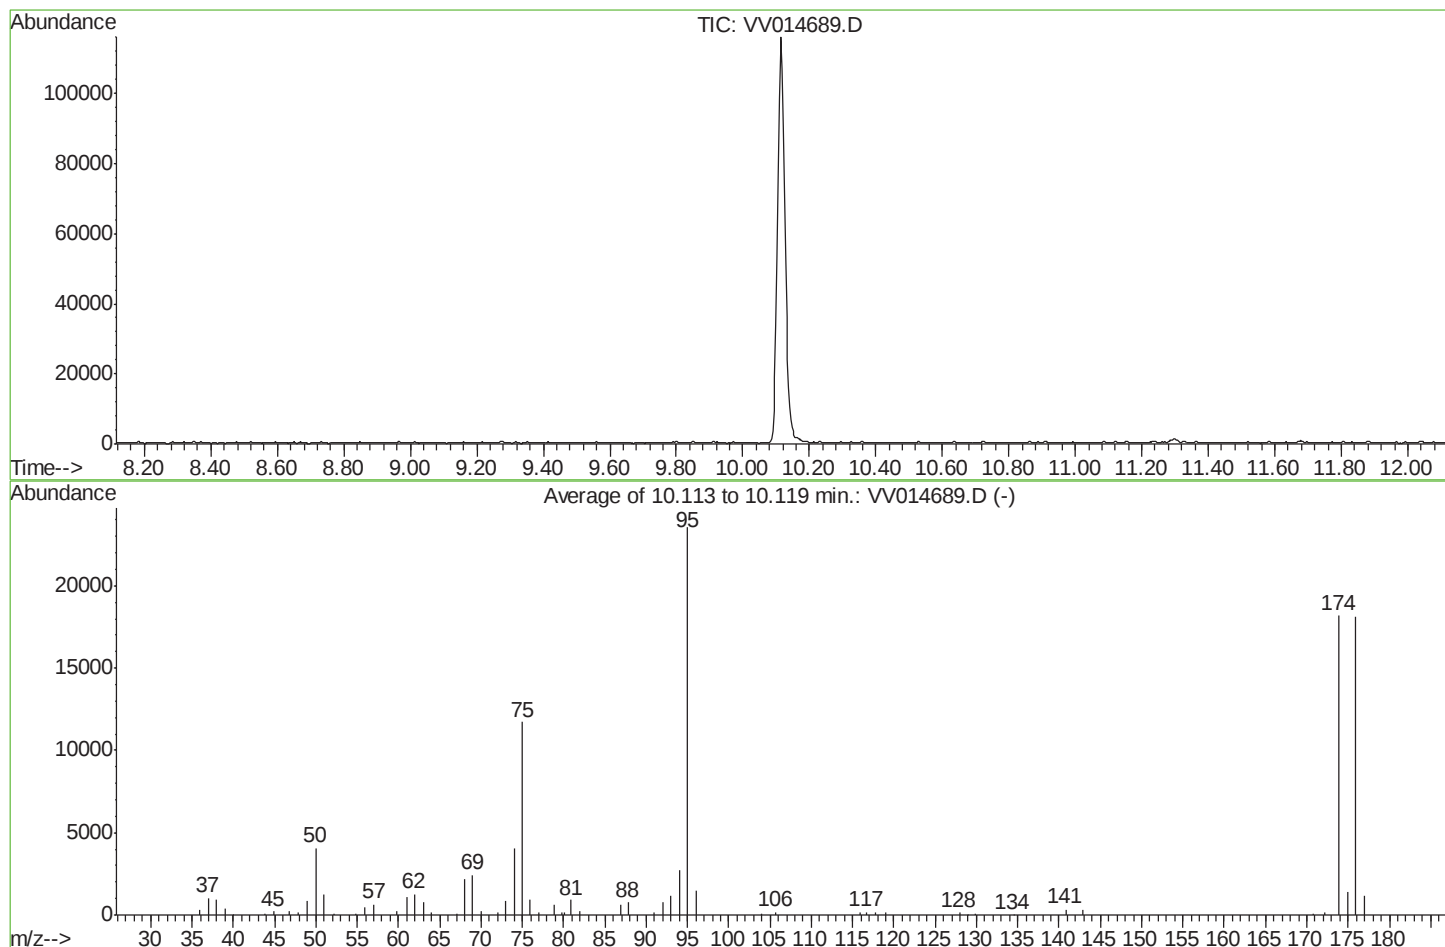

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	4067	PASS
75	95	30	80	49.8	11721	PASS
95	95	100	100	100.0	23549	PASS
96	95	5	9	6.3	1489	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.2	18178	PASS
175	174	5	9	7.9	1434	PASS
176	174	95	101	99.8	18138	PASS
177	176	5	9	6.3	1136	PASS

Scan 2795 (10.077 min): VV014689.D
BFB95

m/z	Abundance
39.90	128.0
42.00	107.0
44.00	143.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95

m/z	Abundance
35.90	284.0
37.00	1032.0
38.00	977.0
39.00	421.0
40.00	179.0
43.90	259.0
44.90	189.0
46.80	245.0
47.90	205.0
49.00	938.0
50.00	4440.0
51.00	1259.0
52.20	110.0
54.80	120.0
55.90	465.0
57.00	667.0
59.90	242.0
61.00	1108.0
61.90	1319.0
63.00	806.0
63.90	171.0
67.00	125.0
68.00	2276.0
69.00	2430.0
70.00	260.0
72.00	184.0
72.90	848.0
74.00	4180.0
75.00	11757.0
76.00	1028.0
77.10	172.0
78.80	669.0
80.20	234.0
80.90	914.0
81.90	221.0
86.90	684.0
87.80	868.0
91.00	169.0
92.00	767.0
93.00	1224.0
94.00	2690.0
95.00	23784.0
96.00	1499.0
105.70	188.0
115.90	140.0
116.80	196.0
117.70	121.0
119.00	151.0
127.90	130.0
128.90	120.0
129.80	119.0
140.80	338.0
142.90	325.0
172.10	182.0
173.90	18024.0
174.90	1519.0
175.90	17576.0
176.90	1149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95

m/z	Abundance
35.80	308.0
37.00	1095.0
38.00	940.0
39.00	393.0
39.90	154.0
43.90	250.0
44.90	229.0
46.80	253.0
47.80	176.0
49.00	901.0
50.00	4182.0
51.00	1259.0
52.10	102.0
54.80	115.0
55.90	492.0
57.10	648.0
59.80	203.0
61.00	1151.0
61.90	1302.0
63.00	805.0
63.90	150.0
67.00	102.0
68.00	2202.0
69.00	2544.0
70.00	247.0
72.00	153.0
72.90	870.0
74.00	4216.0
75.00	12172.0
76.00	935.0
77.00	176.0
78.90	642.0
79.80	232.0
80.10	215.0
80.90	940.0
81.90	252.0
86.90	627.0
87.90	776.0
91.00	206.0
92.00	803.0
93.00	1228.0
94.00	2830.0
95.00	24256.0
96.00	1529.0
103.90	120.0
105.70	190.0
115.90	156.0
116.80	199.0
117.70	166.0
119.00	162.0
128.00	135.0
129.80	113.0
134.50	105.0
140.80	373.0
142.90	368.0
170.80	108.0
172.20	171.0
173.90	18944.0
174.90	1476.0
175.90	18944.0
176.90	1165.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95

m/z	Abundance
35.80	265.0
37.00	1015.0
38.00	819.0
39.00	324.0
39.90	139.0
43.80	264.0
44.90	258.0
46.80	223.0
47.80	172.0
48.90	832.0
50.00	3579.0
51.00	1190.0
54.90	101.0
56.00	438.0
57.10	572.0
59.80	175.0
61.00	1111.0
61.90	1124.0
63.00	782.0
63.90	116.0
68.00	1969.0
69.00	2269.0
70.00	197.0
72.00	146.0
73.00	843.0
74.00	3805.0
75.00	11236.0
75.90	828.0
77.00	166.0
79.00	655.0
79.80	237.0
80.90	884.0
82.00	240.0
87.00	670.0
87.90	654.0
91.00	208.0
92.00	673.0
93.00	1111.0
94.00	2647.0
95.00	22608.0
96.00	1439.0
103.90	149.0
105.70	147.0
115.80	168.0
116.70	185.0
117.70	182.0
118.90	150.0
127.90	125.0
129.90	108.0
140.80	342.0
142.90	348.0
170.80	124.0
172.10	156.0
173.90	17568.0
174.90	1307.0
175.90	17896.0
176.90	1096.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95