
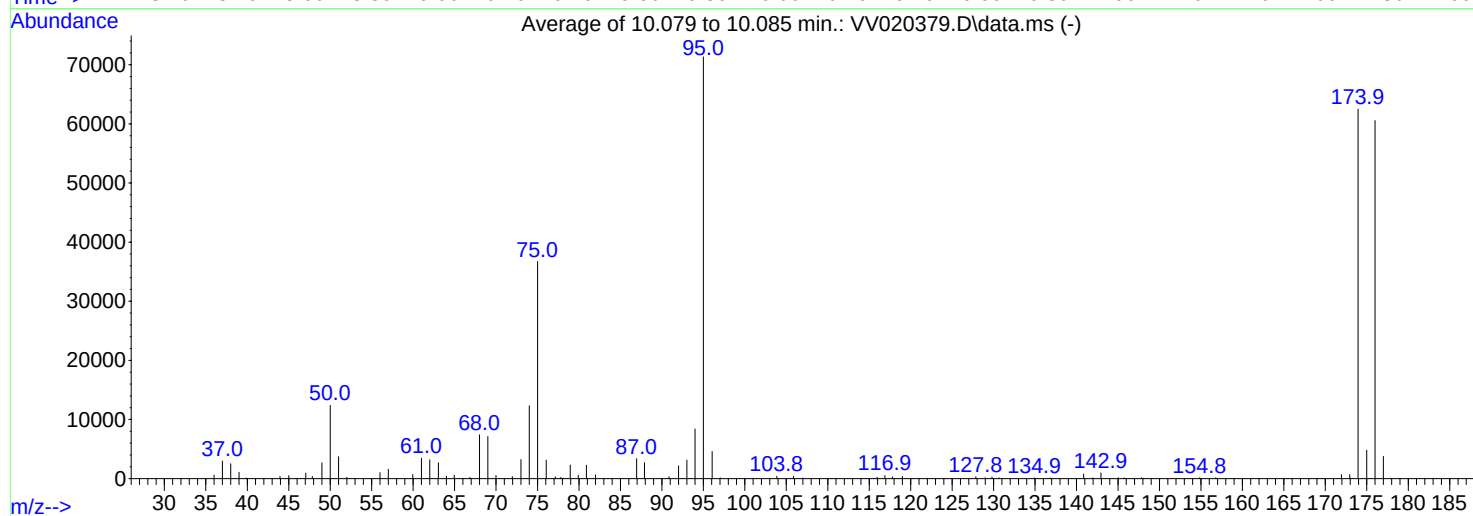


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022421\
 Data File : VV020379.D
 Acq On : 23 Feb 2021 13:43
 Operator : SY/MD
 Sample : BFB85
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB8701

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022421WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Feb 24 03:03:54 2021

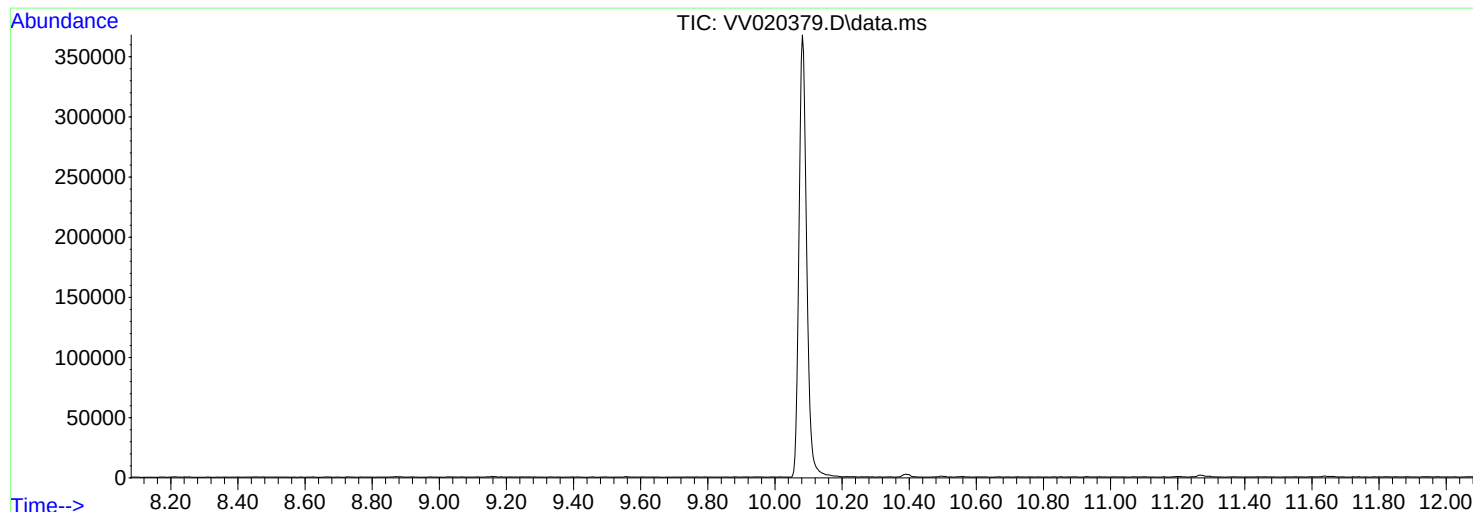

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	12403	PASS
75	95	30	80	51.5	36728	PASS
95	95	100	100	100.0	71333	PASS
96	95	5	9	6.5	4604	PASS
173	174	0.00	2	1.1	671	PASS
174	95	50	120	87.6	62504	PASS
175	174	5	9	7.7	4819	PASS
176	174	95	105	96.9	60568	PASS
177	176	5	10	6.2	3771	PASS

m/z	Abundance
36.00	630.0
37.00	2944.0
38.00	2491.0
39.00	1138.0
39.90	213.0
44.00	905.0
45.00	451.0
47.10	1059.0
47.80	356.0
49.00	2840.0
50.00	12533.0
51.00	3703.0
52.00	237.0
54.90	111.0
56.00	985.0
57.00	1568.0
59.90	727.0
61.00	3431.0
62.00	3163.0
63.00	2681.0
64.00	384.0
64.90	502.0
66.00	101.0
66.80	153.0
68.00	7300.0
69.00	7124.0
70.00	488.0
72.00	342.0
73.00	3185.0
74.00	12251.0
75.00	36080.0
76.00	3218.0
77.20	299.0
77.80	325.0
79.00	2299.0
79.90	525.0
80.90	2318.0
82.00	634.0
86.90	3147.0
87.90	2597.0
90.90	331.0
92.00	2006.0
93.00	3004.0
94.00	8375.0
95.00	69632.0
96.10	4685.0
97.00	159.0
103.80	351.0
105.80	384.0
107.10	123.0
116.00	242.0
116.90	524.0
117.80	288.0
119.00	395.0
127.80	309.0
129.00	141.0
129.80	269.0
130.70	107.0
135.00	127.0
136.80	105.0
140.80	758.0
142.00	140.0
142.90	909.0
145.10	176.0
145.80	160.0
147.90	138.0
148.10	141.0
154.90	135.0
156.80	159.0
172.00	693.0
173.00	705.0
174.00	59920.0
175.00	4697.0
176.00	57168.0
177.00	3655.0

Instrument :
MSVOA_V
ClientSampleId :
BFB8701

m/z	Abundance
36.00	639.0
37.00	3118.0
38.00	2592.0
39.00	1139.0
39.90	274.0
44.00	913.0
45.00	540.0
47.10	1006.0
47.90	386.0
49.00	2735.0
50.00	12810.0
51.00	3827.0
52.00	235.0
56.00	1030.0
57.00	1597.0
59.90	727.0
61.00	3547.0
62.00	3228.0
63.00	2766.0
64.00	446.0
65.00	615.0
66.80	231.0
68.00	7735.0
69.00	7350.0
70.00	529.0
72.00	370.0
73.00	3348.0
74.00	12754.0
75.00	38120.0
76.00	3230.0
77.20	310.0
77.80	290.0
79.00	2349.0
79.90	594.0
80.90	2333.0
82.00	653.0
86.90	3545.0
87.90	2887.0
90.90	326.0
92.00	2227.0
93.00	3238.0
94.00	8655.0
95.00	73624.0
96.00	4766.0
97.00	136.0
103.80	427.0
105.90	425.0
107.00	118.0
115.90	247.0
116.90	573.0
117.80	294.0
119.00	381.0
127.80	328.0
129.00	167.0
129.80	275.0
130.70	133.0
135.00	150.0
136.80	126.0
140.90	793.0
141.90	131.0
143.00	1042.0
145.10	180.0
145.80	135.0
147.80	186.0
154.90	157.0
156.80	165.0
172.00	690.0
173.00	699.0
173.90	64608.0
175.00	5051.0
176.00	62816.0
177.00	3849.0
177.90	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB8701

m/z	Abundance
36.00	541.0
37.00	2910.0
38.00	2503.0
39.00	955.0
39.90	310.0
44.00	863.0
45.00	570.0
47.00	806.0
47.90	390.0
49.00	2465.0
50.00	11865.0
51.00	3631.0
52.00	211.0
56.00	1069.0
57.00	1620.0
58.00	122.0
60.00	642.0
61.00	3349.0
62.00	3165.0
63.10	2607.0
64.00	474.0
65.00	678.0
66.90	276.0
68.00	7214.0
69.00	6859.0
70.00	592.0
71.90	356.0
73.00	3149.0
74.00	12058.0
75.00	35984.0
76.10	2943.0
77.10	331.0
78.10	247.0
78.90	2215.0
79.90	639.0
80.90	2200.0
82.00	606.0
87.00	3461.0
87.90	2658.0
90.80	294.0
92.00	2249.0
93.00	3151.0
94.00	8251.0
95.00	70744.0
96.00	4362.0
97.10	108.0
103.90	465.0
105.90	395.0
106.90	110.0
115.90	284.0
116.90	561.0
117.80	320.0
119.00	388.0
127.90	325.0
129.00	177.0
129.80	247.0
130.60	133.0
134.90	124.0
136.80	121.0
140.90	829.0
141.90	119.0
143.00	953.0
145.00	157.0
145.70	127.0
146.80	106.0
147.80	213.0
154.80	233.0
156.80	145.0
171.90	649.0
172.90	609.0
173.90	62984.0
175.00	4708.0
176.00	61720.0
177.00	3809.0
177.90	162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB8701

m/z	Abundance
39.90	167.0
43.90	521.0

Instrument :
MSVOA_V
ClientSampleId :
BFB8701