

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022424\
 Data File : VW034392.D
 Acq On : 24 Feb 2024 13:24
 Operator : SY/MD
 Sample : P1498-18DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC2DL

Quant Time: Feb 26 00:36:32 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Feb 24 00:41:32 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	80128	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	74224	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	37496	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	32819	5.289	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	105.800%	
7) Chloroethane-d5	1.535	69	25761	4.739	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	94.800%	
11) 1,1-Dichloroethene-d2	2.059	65	14355	4.797	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	96.000%	
20) 2-Butanone-d5	3.805	46	45710	43.858	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	87.720%	
24) Chloroform-d	4.252	84	54651	4.846	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.000%	
26) 1,2-Dichloroethane-d4	4.947	65	26606	5.049	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	101.000%	
32) Benzene-d6	4.963	84	104003	4.670	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.400%	
36) 1,2-Dichloropropane-d6	5.992	67	30265	4.862	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	97.200%	
41) Toluene-d8	7.246	98	96053	4.693	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	93.800%	
43) trans-1,3-Dichloroprop...	7.561	79	7313	3.111	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	62.200%	
46) 2-Hexanone-d5	8.027	63	38280	45.621	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	91.240%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	18906	5.010	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	100.200%	
66) 1,2-Dichlorobenzene-d4	11.561	152	33314	4.885	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	97.800%	
Target Compounds						
12) 1,1-Dichloroethene	2.072	96	4087	0.730	ug/L #	1
14) Carbon disulfide	2.246	76	2418	0.134	ug/L #	74
22) cis-1,2-Dichloroethene	3.825	96	2314	0.358	ug/L	98
34) Trichloroethene	5.834	95	55595	8.629	ug/L	99
47) Tetrachloroethene	7.915	164	1240	0.237	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022424\
Data File : VV034392.D
Acq On : 24 Feb 2024 13:24
Operator : SY/MD
Sample : P1498-18DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC2DL

Quant Time: Feb 26 00:36:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Feb 24 00:41:32 2024
Response via : Initial Calibration

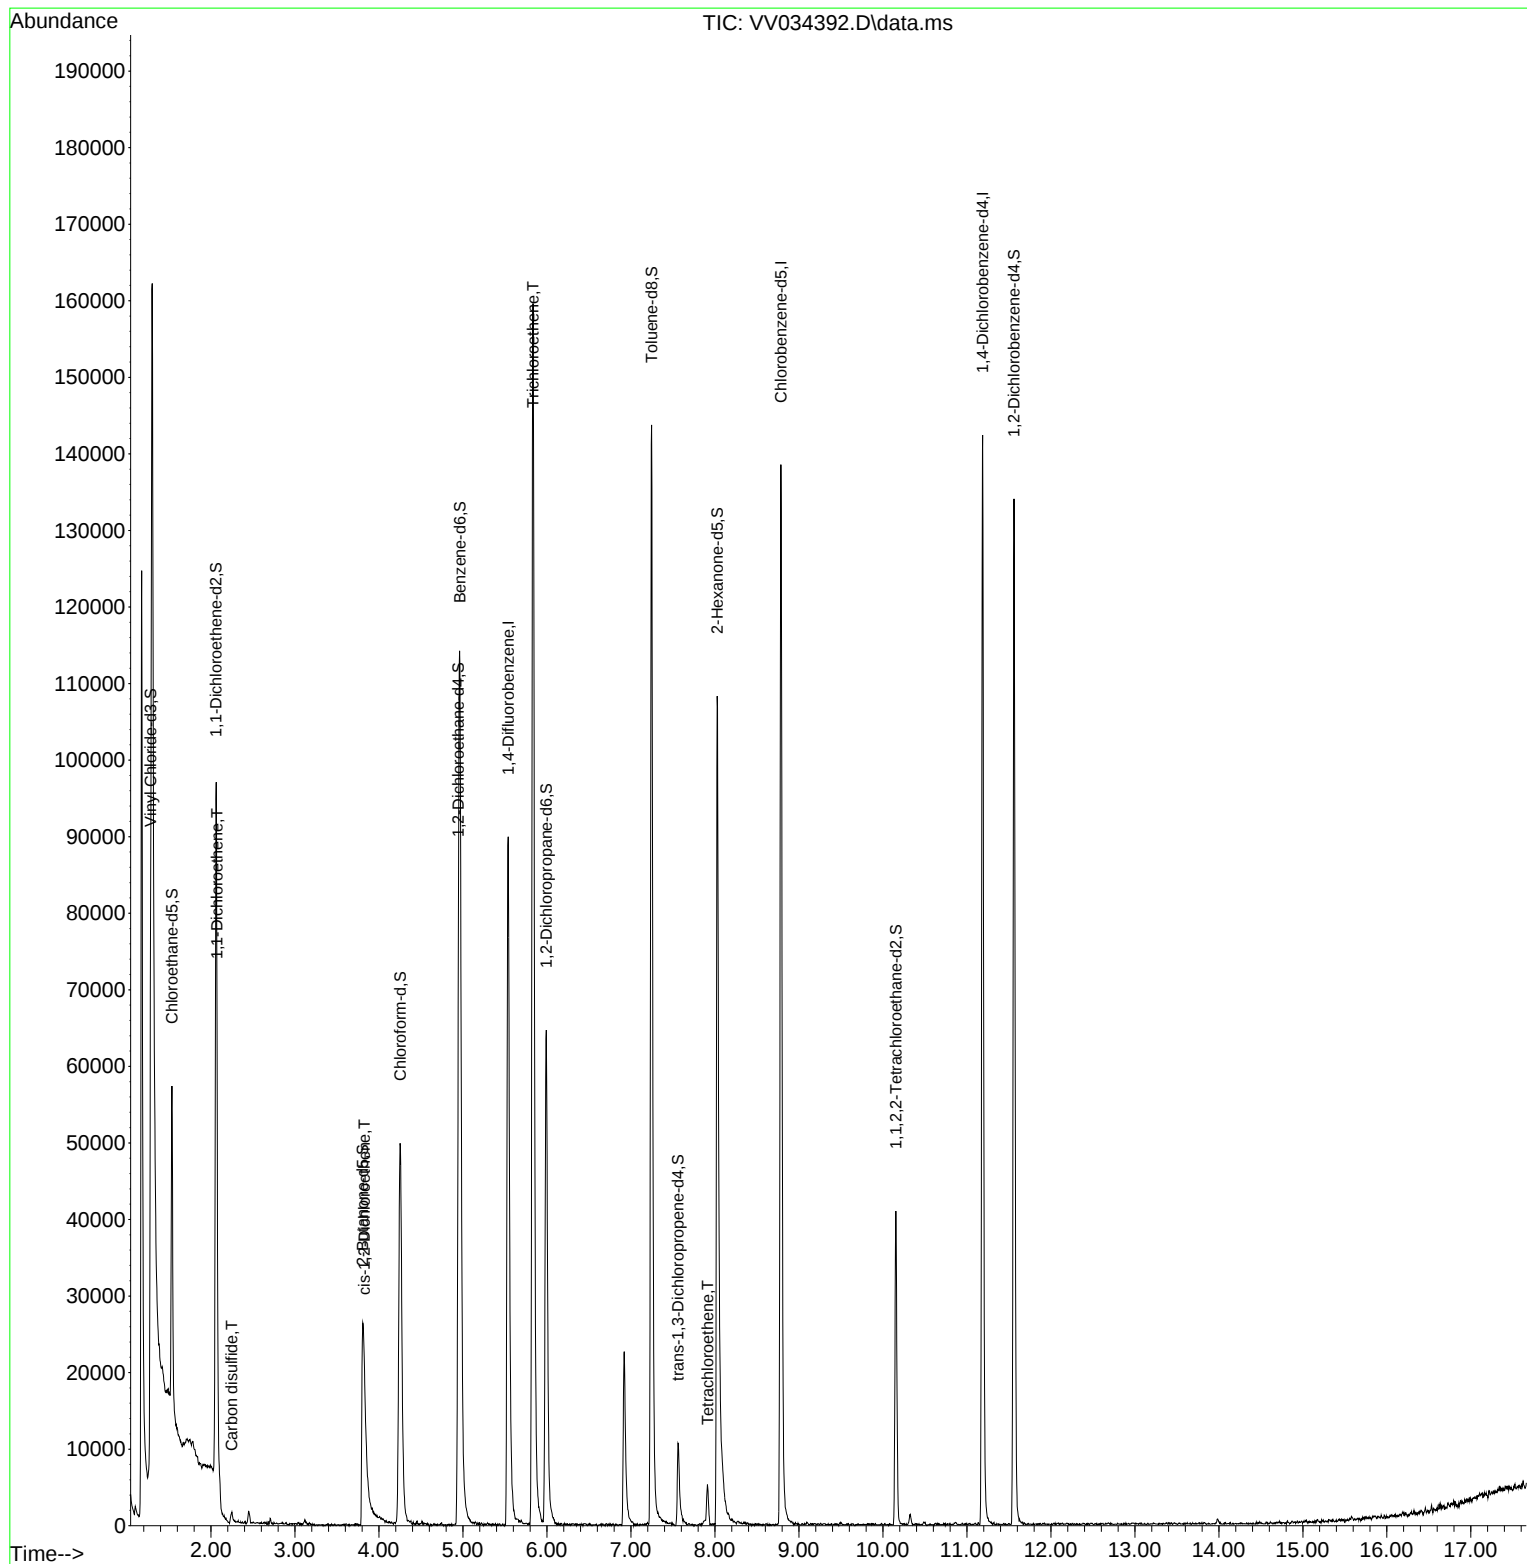

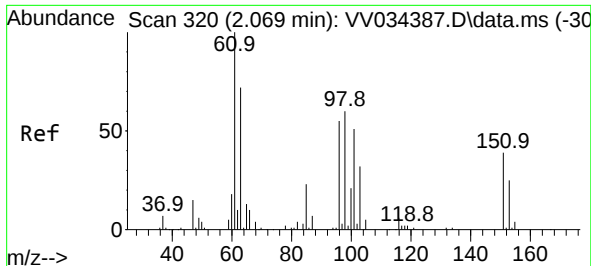

#12

1,1-Dichloroethene

Concen: 0.730 ug/L

RT: 2.072 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV034392.D

Acq: 24 Feb 2024 13:24

Instrument :

MSVOA_V

ClientSampleId :

C0AC2DL





Tgt Ion: 96 Resp: 4087

Ion Ratio Lower Upper

96 100

61 237.2 128.8 239.2

63 616.7 97.9 181.9#

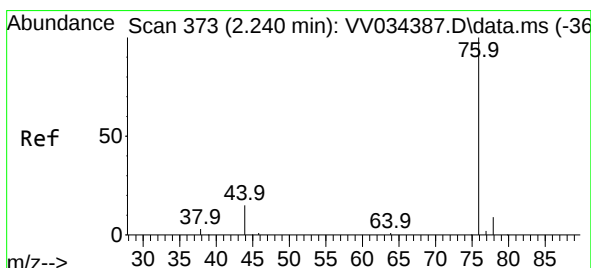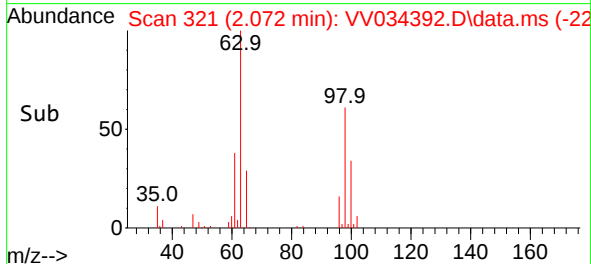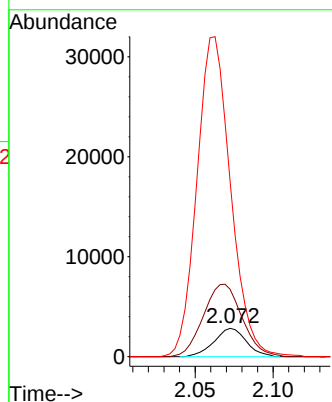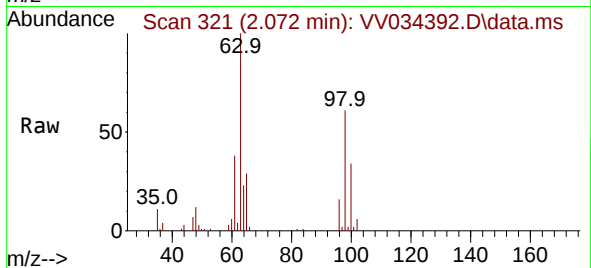

#14

Carbon disulfide

Concen: 0.134 ug/L

RT: 2.246 min Scan# 375

Delta R.T. 0.006 min

Lab File: VV034392.D




Acq: 24 Feb 2024 13:24


Tgt Ion: 76 Resp: 2418

Ion Ratio Lower Upper

76 100

78 0.0 7.5 11.3#

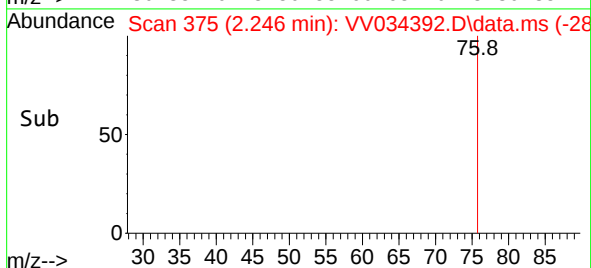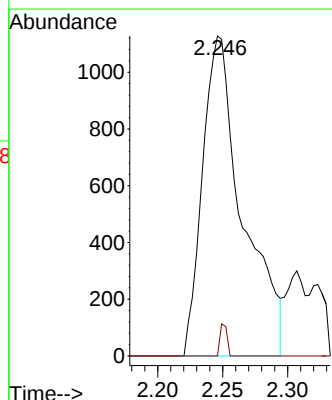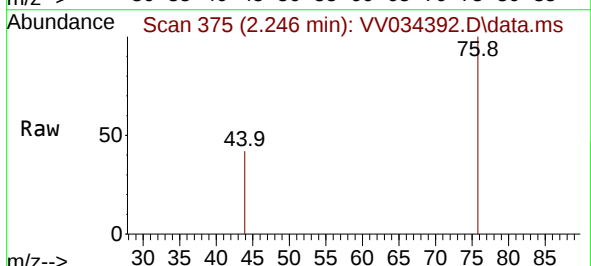

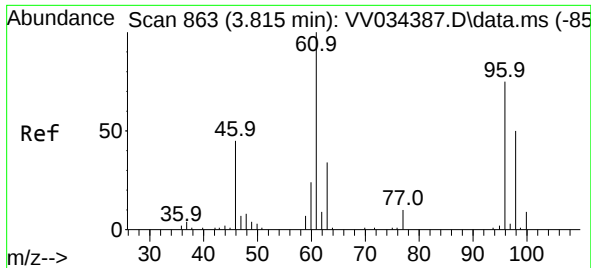

#22

cis-1,2-Dichloroethene

Concen: 0.358 ug/L

RT: 3.825 min Scan# 866

Delta R.T. 0.009 min

Lab File: VV034392.D

Acq: 24 Feb 2024 13:24

Instrument :

MSVOA_V

ClientSampleId :

C0AC2DL





Tgt Ion: 96 Resp: 2314

Ion Ratio Lower Upper

96 100

61 130.6 90.3 167.7

98 63.4 43.2 80.2

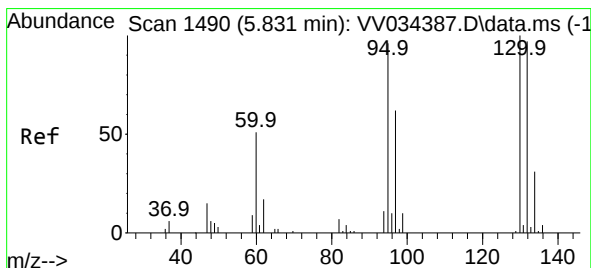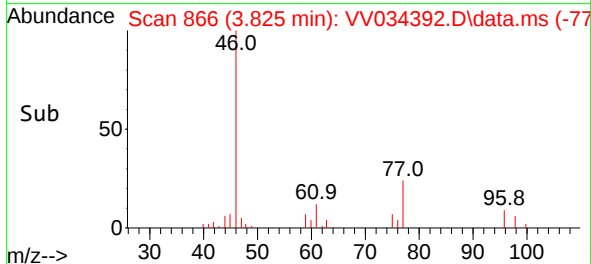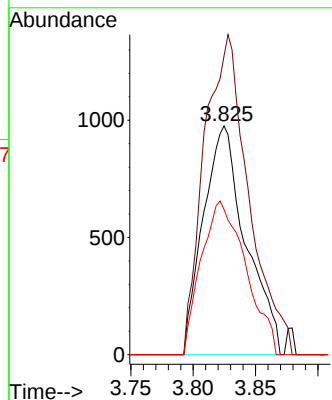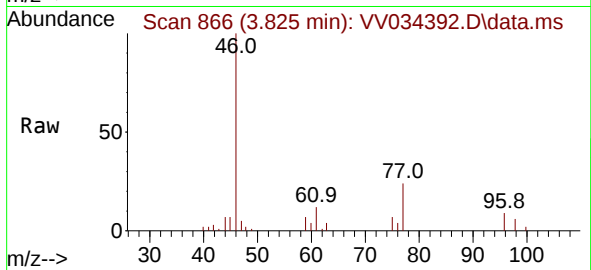

#34

Trichloroethene

Concen: 8.629 ug/L

RT: 5.834 min Scan# 1491

Delta R.T. -0.000 min

Lab File: VV034392.D

Acq: 24 Feb 2024 13:24

Tgt Ion: 95 Resp: 55595




Ion Ratio Lower Upper


95 100

97 64.3 45.1 83.7

132 95.9 66.0 122.6

130 101.3 72.2 134.0

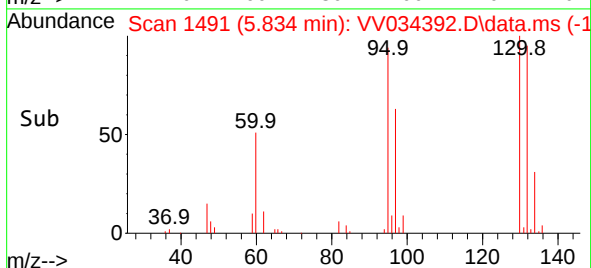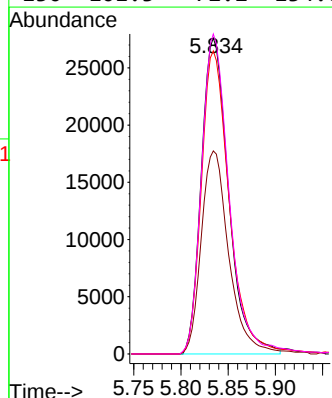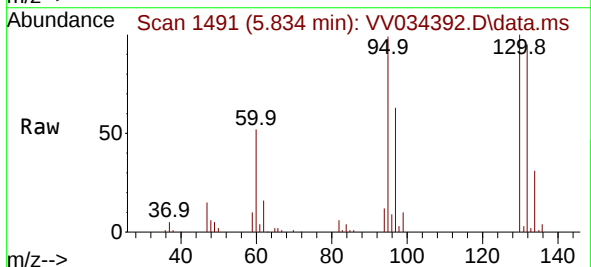

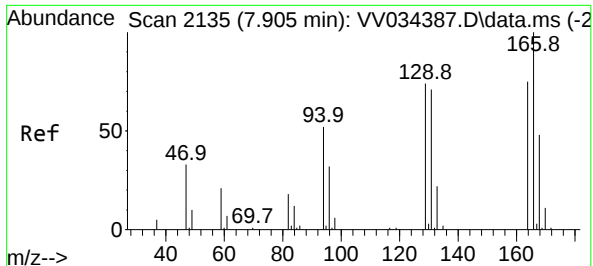

#47
Tetrachloroethene
Concen: 0.237 ug/L
RT: 7.915 min Scan# 21
Delta R.T. 0.009 min
Lab File: VV034392.D
Acq: 24 Feb 2024 13:24

Instrument :
MSVOA_V
ClientSampleId :
C0AC2DL

Tgt Ion:164 Resp: 1240

Ion	Ratio	Lower	Upper
164	100		
129	82.6	67.8	125.8
131	77.5	63.0	117.0
166	123.8	92.6	172.0

