


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022424\
Data File : VV034386.D
Acq On : 24 Feb 2024 09:39
Operator : SY/MD
Sample : BFB260
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB260

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Feb 24 00:41:32 2024

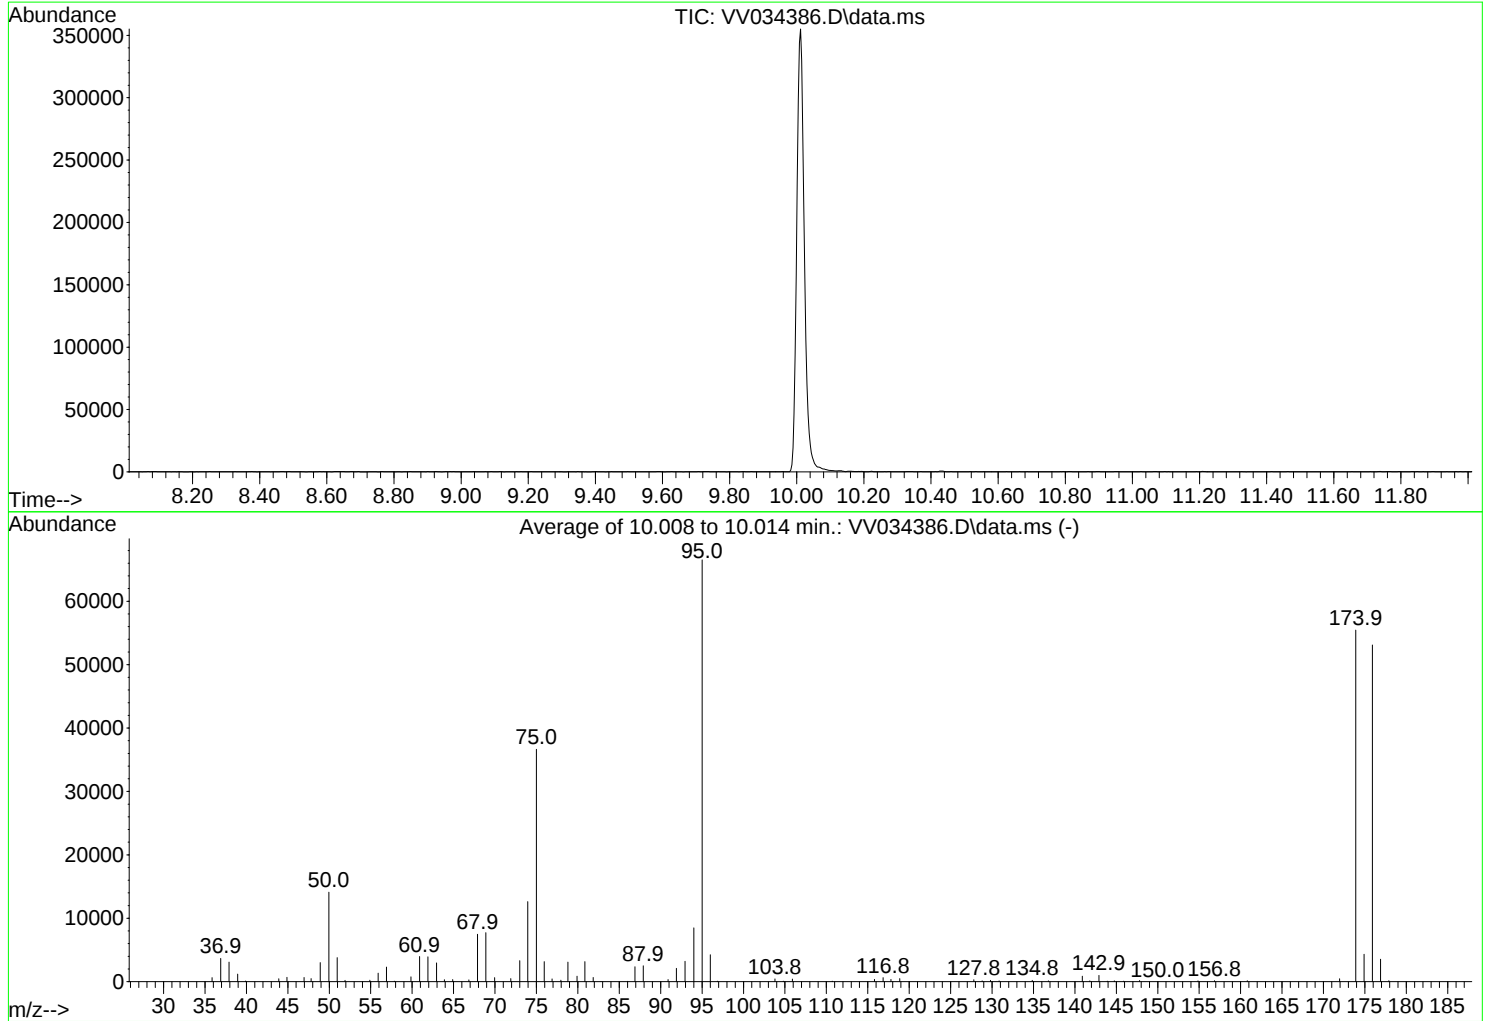

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	14105	PASS
75	95	30	80	55.1	36648	PASS
95	95	100	100	100.0	66531	PASS
96	95	5	9	6.4	4231	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.4	55459	PASS
175	174	5	9	7.8	4315	PASS
176	174	95	105	95.8	53107	PASS
177	176	5	10	6.7	3534	PASS

m/z	Abundance
43.90	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB260

m/z	Abundance
35.90	679.0
36.90	3697.0
37.90	3252.0
38.90	1130.0
39.90	107.0
43.90	613.0
44.90	636.0
47.00	689.0
47.80	511.0
48.90	3097.0
49.90	14628.0
50.90	3908.0
51.90	219.0
54.90	276.0
55.90	1441.0
56.90	2320.0
59.80	749.0
60.90	3974.0
61.90	3984.0
62.90	3043.0
63.90	327.0
64.90	339.0
66.90	308.0
67.90	7597.0
68.90	7865.0
70.00	627.0
71.90	477.0
73.00	3488.0
73.90	12629.0
75.00	37232.0
76.00	3241.0
76.90	449.0
77.90	202.0
78.80	3174.0
79.90	850.0
80.80	3129.0
81.80	712.0
82.80	111.0
86.00	130.0
86.90	2322.0
87.90	2512.0
90.90	354.0
91.90	2161.0
92.90	3221.0
94.00	8341.0
95.00	67256.0
96.00	4376.0
96.90	101.0
103.80	452.0
104.80	117.0
105.90	378.0
110.70	128.0
115.80	327.0
116.80	609.0
117.80	375.0
118.80	522.0
127.80	315.0
128.80	120.0
129.80	189.0
130.80	152.0
134.80	239.0
136.80	139.0
140.90	880.0
141.80	115.0
142.90	951.0
143.90	121.0
144.80	130.0
147.80	159.0
154.80	140.0
156.90	163.0
160.80	162.0
172.00	476.0
173.90	54400.0
174.90	4342.0
175.90	51728.0
176.90	3492.0
177.90	136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB260

m/z	Abundance
35.80	661.0
36.90	3820.0
37.90	3210.0
39.00	1222.0
39.90	114.0
44.00	586.0
44.90	718.0
46.90	719.0
47.80	504.0
48.90	3104.0
50.00	14632.0
50.90	3925.0
51.90	216.0
54.90	234.0
55.90	1401.0
56.90	2394.0
57.90	102.0
59.90	802.0
60.90	4150.0
61.90	4074.0
63.00	3041.0
63.90	314.0
64.90	347.0
66.90	287.0
67.90	7704.0
68.90	7978.0
70.00	648.0
71.90	515.0
73.00	3446.0
74.00	13015.0
75.00	37952.0
76.00	3267.0
76.90	456.0
78.00	231.0
78.80	3200.0
79.90	894.0
80.80	3225.0
81.80	673.0
86.90	2417.0
87.90	2588.0
90.90	343.0
91.90	2134.0
93.00	3363.0
94.00	8777.0
95.00	69128.0
96.00	4361.0
96.80	111.0
103.80	469.0
104.80	116.0
105.90	413.0
110.70	120.0
115.80	376.0
116.90	680.0
117.80	353.0
118.80	508.0
127.80	327.0
128.80	128.0
129.80	198.0
130.90	132.0
134.80	228.0
136.80	117.0
140.90	892.0
141.80	132.0
142.90	1035.0
143.90	112.0
144.70	152.0
145.90	108.0
147.80	173.0
154.80	133.0
156.80	174.0
160.80	179.0
172.00	463.0
173.90	57384.0
174.90	4441.0
175.90	54712.0
176.90	3680.0
177.90	144.0

Instrument :
MSVOA_V
ClientSampleId :
BFB260

m/z	Abundance
35.90	581.0
36.90	3468.0
37.90	2799.0
39.00	1181.0
39.90	122.0
44.00	581.0
44.90	704.0
46.90	602.0
47.80	460.0
48.90	2823.0
50.00	13055.0
51.00	3553.0
51.90	200.0
54.90	197.0
55.90	1189.0
56.90	2164.0
57.80	110.0
59.90	738.0
60.90	3789.0
61.90	3707.0
62.90	2808.0
63.90	275.0
64.90	315.0
66.80	246.0
67.90	7105.0
68.90	7358.0
69.90	632.0
71.90	435.0
73.00	3024.0
74.00	12224.0
75.00	34760.0
75.90	2958.0
76.90	400.0
78.00	227.0
78.80	2896.0
79.90	853.0
80.90	3078.0
81.90	586.0
86.90	2288.0
87.90	2426.0
90.90	313.0
91.90	1993.0
92.90	3041.0
94.00	8315.0
95.00	63208.0
96.00	3957.0
103.80	396.0
105.90	413.0
115.80	373.0
116.90	642.0
117.80	318.0
118.90	423.0
127.80	308.0
128.80	131.0
129.80	204.0
130.90	119.0
134.90	175.0
136.80	116.0
140.90	799.0
141.80	102.0
142.90	996.0
144.70	126.0
145.90	106.0
147.80	176.0
150.00	102.0
154.90	142.0
156.80	152.0
160.80	139.0
171.90	419.0
173.90	54592.0
174.90	4161.0
175.90	52880.0
176.90	3431.0
177.90	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB260