


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022519\
Data File : VV009344.D
Acq On : 25 Feb 2019 09:12
Operator : SY/MD
Sample : BFB66
Misc : 5.00G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB66

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM022019S.M
Title : VOC Analysis
Last Update : Tue Feb 26 02:46:42 2019

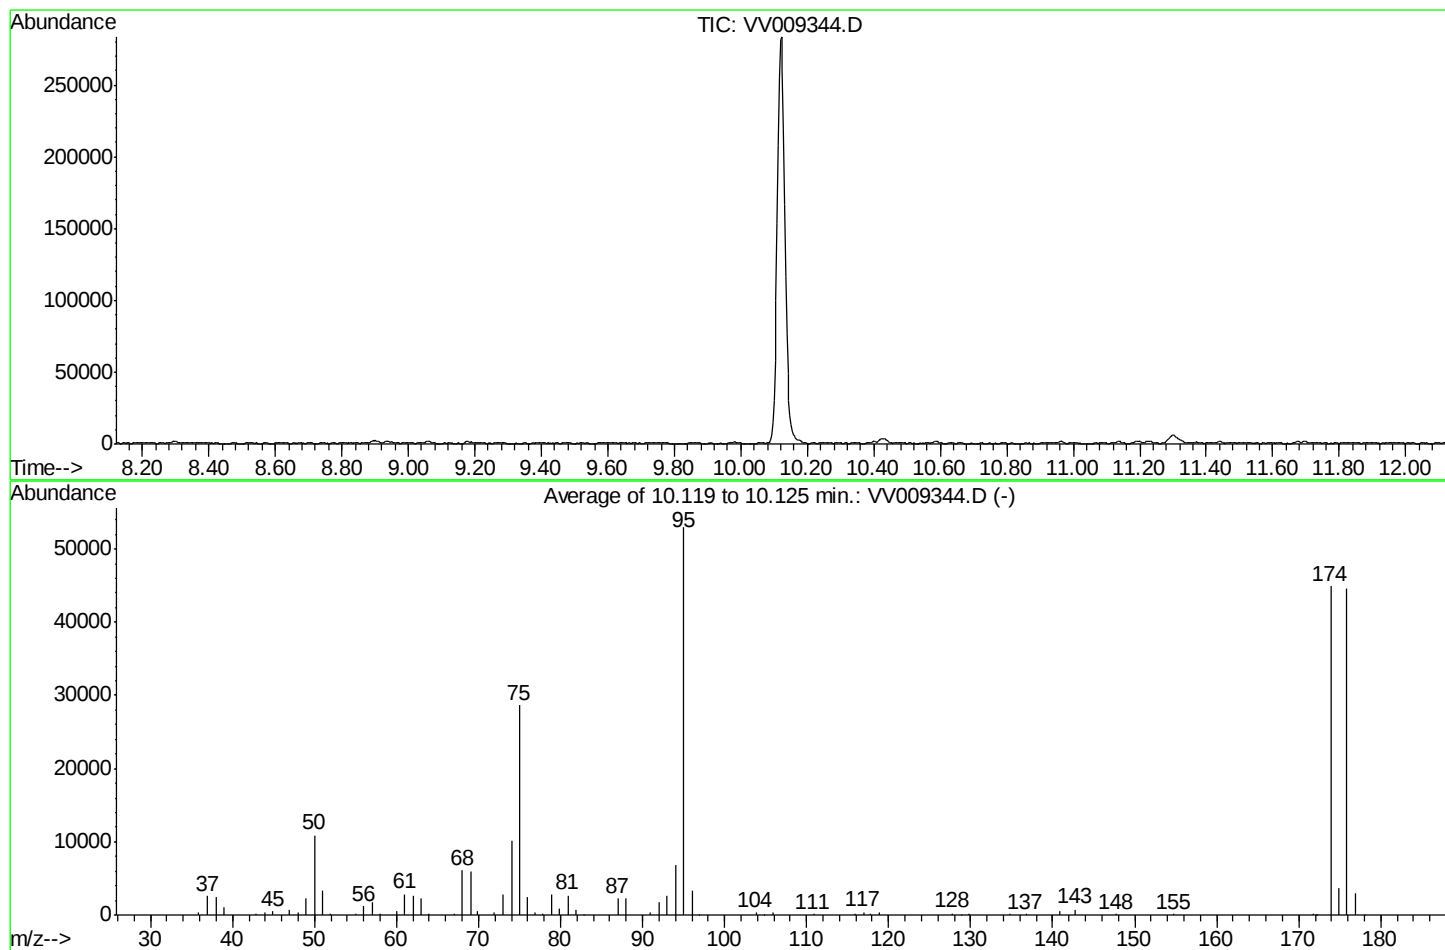

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	10881	PASS
75	95	30	80	54.1	28642	PASS
95	95	100	100	100.0	52960	PASS
96	95	5	9	6.2	3298	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.7	44864	PASS
175	174	5	9	8.0	3610	PASS
176	174	95	101	99.5	44645	PASS
177	176	5	9	6.8	3029	PASS

m/z	Abundance
36.00	384.0
37.00	2656.0
38.00	2524.0
39.00	1134.0
39.90	166.0
43.00	155.0
44.00	618.0
44.90	501.0
46.90	787.0
47.90	337.0
49.00	2279.0
50.00	11620.0
51.00	3551.0
51.90	206.0
55.10	245.0
56.00	1162.0
57.00	1982.0
58.10	141.0
59.90	671.0
61.00	2885.0
62.00	2727.0
63.00	2302.0
63.90	180.0
67.00	179.0
68.00	6197.0
69.00	6270.0
69.90	598.0
71.90	270.0
73.00	2625.0
74.00	10431.0
75.00	29784.0
76.00	2482.0
77.00	341.0
77.70	271.0
78.90	2905.0
79.90	840.0
80.90	2846.0
81.90	642.0
87.00	2363.0
87.90	2232.0
90.80	227.0
92.00	1664.0
92.90	2695.0
94.00	7070.0
95.00	54240.0
96.00	3727.0
96.90	125.0
103.80	362.0
104.90	110.0
105.90	309.0
110.90	137.0
115.90	227.0
117.00	389.0
117.80	280.0
118.80	272.0
127.80	228.0
128.90	156.0
129.90	224.0
134.80	153.0
136.80	133.0
140.90	603.0
142.80	768.0
147.80	116.0
154.80	186.0
171.80	164.0
172.00	163.0
173.90	45136.0
174.90	3637.0
175.90	44144.0
176.90	3137.0
178.00	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

m/z	Abundance
35.90	359.0
37.00	2650.0
38.00	2448.0
39.00	1202.0
39.80	158.0
42.80	145.0
44.00	596.0
45.00	532.0
47.00	747.0
48.00	341.0
49.00	2306.0
50.00	11220.0
51.00	3351.0
51.90	195.0
55.10	241.0
56.00	1208.0
57.00	1836.0
58.10	144.0
60.00	574.0
61.00	2881.0
62.00	2791.0
63.00	2233.0
64.00	192.0
67.00	205.0
68.00	6236.0
69.00	6078.0
69.90	638.0
71.90	326.0
73.00	2842.0
74.00	10503.0
75.00	29496.0
76.00	2492.0
77.00	311.0
77.80	274.0
78.90	2922.0
79.90	853.0
80.90	2779.0
81.90	732.0
86.90	2298.0
87.90	2287.0
90.90	301.0
92.00	1716.0
93.00	2647.0
94.00	6940.0
95.00	54576.0
96.00	3334.0
96.90	103.0
103.80	365.0
104.80	111.0
105.90	332.0
110.90	144.0
115.80	255.0
117.00	431.0
117.80	256.0
118.80	290.0
127.80	269.0
128.90	117.0
129.90	257.0
134.80	141.0
136.80	159.0
140.90	618.0
142.80	732.0
147.80	113.0
154.80	165.0
171.60	131.0
173.90	46128.0
174.90	3712.0
175.90	46224.0
176.90	3144.0
178.00	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

m/z	Abundance
35.80	336.0
37.00	2433.0
38.00	2215.0
39.00	1128.0
39.80	124.0
42.80	150.0
44.00	566.0
45.00	453.0
47.00	579.0
48.00	324.0
49.00	2145.0
50.00	9804.0
51.00	2893.0
51.90	153.0
55.00	257.0
56.00	1125.0
57.00	1608.0
58.00	132.0
60.00	473.0
61.00	2700.0
62.00	2537.0
63.00	2043.0
64.00	208.0
67.00	192.0
68.00	5832.0
69.00	5591.0
69.90	609.0
72.00	307.0
73.00	2758.0
74.00	9563.0
75.00	26648.0
76.00	2240.0
76.90	302.0
77.80	236.0
78.90	2641.0
79.80	772.0
80.90	2500.0
81.90	767.0
82.80	104.0
86.90	1997.0
88.00	2134.0
90.90	376.0
92.00	1671.0
93.00	2503.0
94.00	6372.0
95.00	50064.0
96.00	2835.0
103.80	297.0
105.80	314.0
110.90	149.0
115.80	230.0
116.90	396.0
117.80	198.0
118.80	316.0
127.80	304.0
129.80	242.0
134.90	102.0
136.80	138.0
140.80	585.0
142.80	649.0
147.70	109.0
154.80	146.0
172.20	148.0
173.90	43328.0
174.90	3481.0
175.90	43568.0
176.90	2806.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

m/z	Abundance
38.80	103.0
40.00	167.0
40.90	132.0
43.90	215.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66