

Data File : VV014707.D
Acq On : 25 Feb 2020 12:23
Operator : SY/MD
Sample : L1607-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Feb 26 01:10:49 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 26 01:08:40 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	219900	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	204174	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	96964	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	32699	38.07	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	76.14%
7) Chloroethane-d5	1.59	69	26414	42.44	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	84.88%
11) 1,1-Dichloroethene-d2	2.13	63	54747	34.20	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.40%
21) 2-Butanone-d5	3.95	46	69335	86.85	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	86.85%
24) Chloroform-d	4.40	84	123869	44.05	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.10%
26) 1,2-Dichloroethane-d4	5.08	65	87817	48.85	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.70%
32) Benzene-d6	5.10	84	246843	45.68	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.36%
36) 1,2-Dichloropropane-d6	6.12	67	71313	45.26	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.52%
41) Toluene-d8	7.36	98	234816	45.11	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.22%
43) trans-1,3-Dichloropropene-	7.66	79	40721	46.13	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.26%
47) 2-Hexanone-d5	8.14	63	61539	97.44	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	97.44%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	101504	46.49	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.98%
64) 1,2-Dichlorobenzene-d4	11.67	152	92624	48.82	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.64%

Target Compounds


					Qvalue	
10) 1,1,2-Trichloro-1,2,2-trif	2.13	101	562	0.755	ug/L #	17
25) Chloroform	4.43	83	6087	2.233	ug/L #	74
59) 1,2,3-Trichloropropane	11.29	75	10375	5.954	ug/L #	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV014707.D
Acq On : 25 Feb 2020 12:23
Operator : SY/MD
Sample : L1607-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Feb 26 01:10:49 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 26 01:08:40 2020
Response via : Initial Calibration

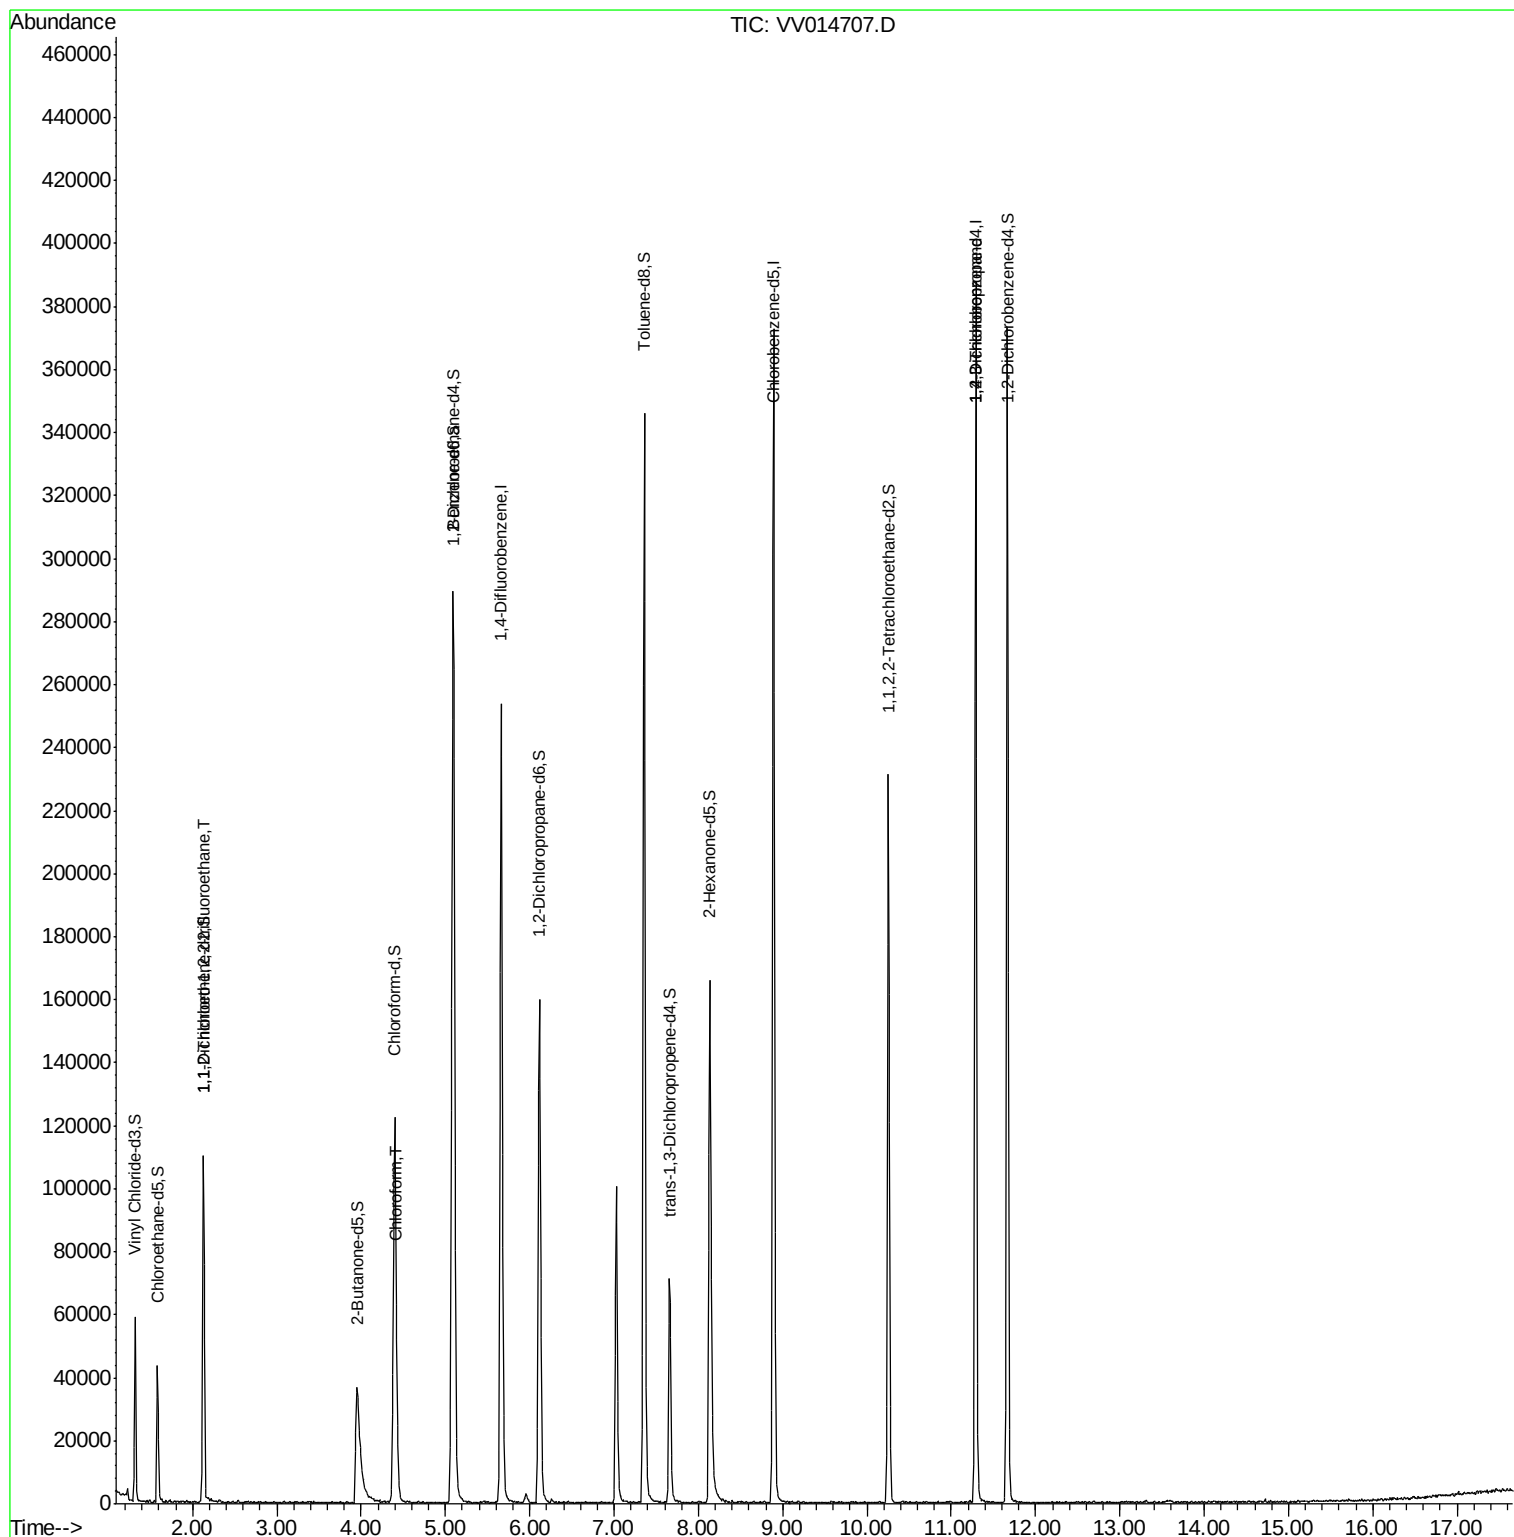

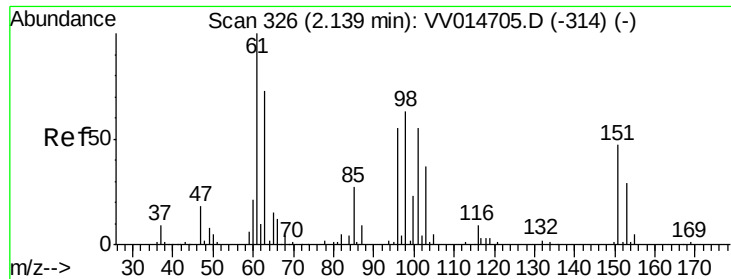

#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 0.755 ug/L

RT: 2.13 min Scan# 322

Delta R.T. -0.01 min

Lab File: VV014707.D

Acq: 25 Feb 2020 12:23

Instrument :

MSVOA_V

ClientSampleId :

VHBLK01


Tgt Ion: 101 Resp: 562

Ion Ratio Lower Upper

101 100

85 0.0 37.3 55.9#

151 0.0 64.6 96.8#

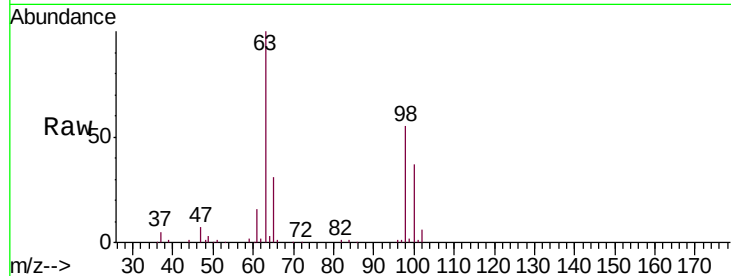

Abundance Ion 101.00 (100.70 to 101.70): V

Ion 85.00 (84.70 to 85.70): VV0

Ion 151.00 (150.70 to 151.70): V

2.13

400

300



200

100

0

2.10 2.12 2.14

Time-->

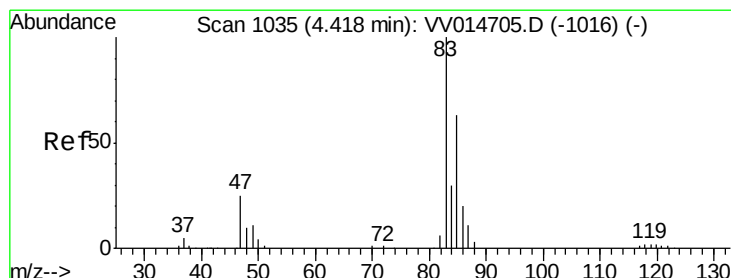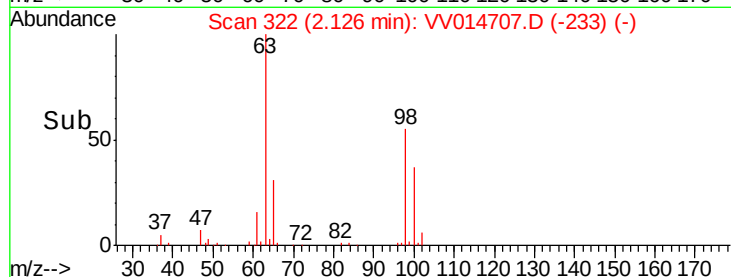

#25

Chloroform

Concen: 2.233 ug/L

RT: 4.43 min Scan# 1038

Delta R.T. 0.01 min

Lab File: VV014707.D


Acq: 25 Feb 2020 12:23

Tgt Ion: 83 Resp: 6087

Ion Ratio Lower Upper

83 100

85 86.3 46.1 85.7#

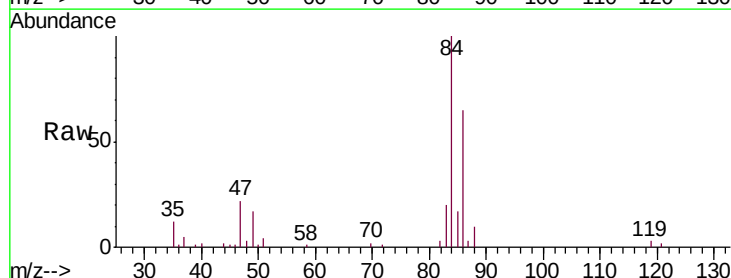

Abundance Ion 83.00 (82.70 to 83.70): VV0

Ion 85.00 (84.70 to 85.70): VV0

2500

2000

1500


1000


500

0

4.35 4.40 4.45 4.50

Time-->

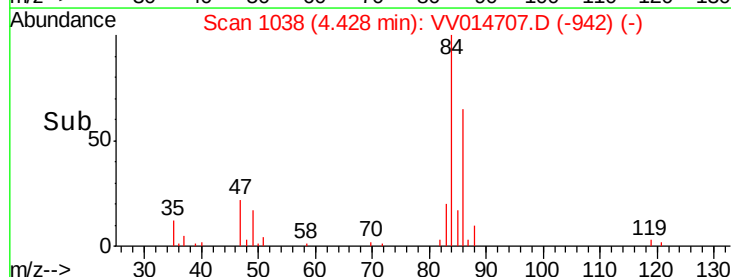

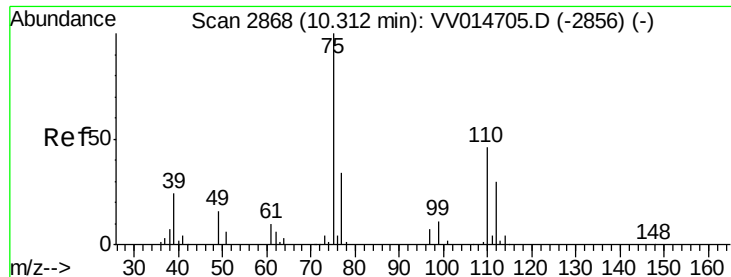

#59

1,2,3-Trichloropropane

Concen: 5.954 ug/L

RT: 11.29 min Scan# 3172

Delta R.T. 0.98 min

Lab File: VV014707.D

Acq: 25 Feb 2020 12:23

Instrument :

MSVOA_V

ClientSampleId :

VHBLK01

Tgt Ion: 75 Resp: 10375

Ion Ratio Lower Upper

75 100

77 40.1 25.7 38.5#

