


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV022520\
 Data File : VV014704.D
 Acq On : 25 Feb 2020 09:32
 Operator : SY/MD
 Sample : BFB96
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB96

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM022120WMA.M
 Title : VOC Analysis
 Last Update : Wed Feb 26 01:08:40 2020

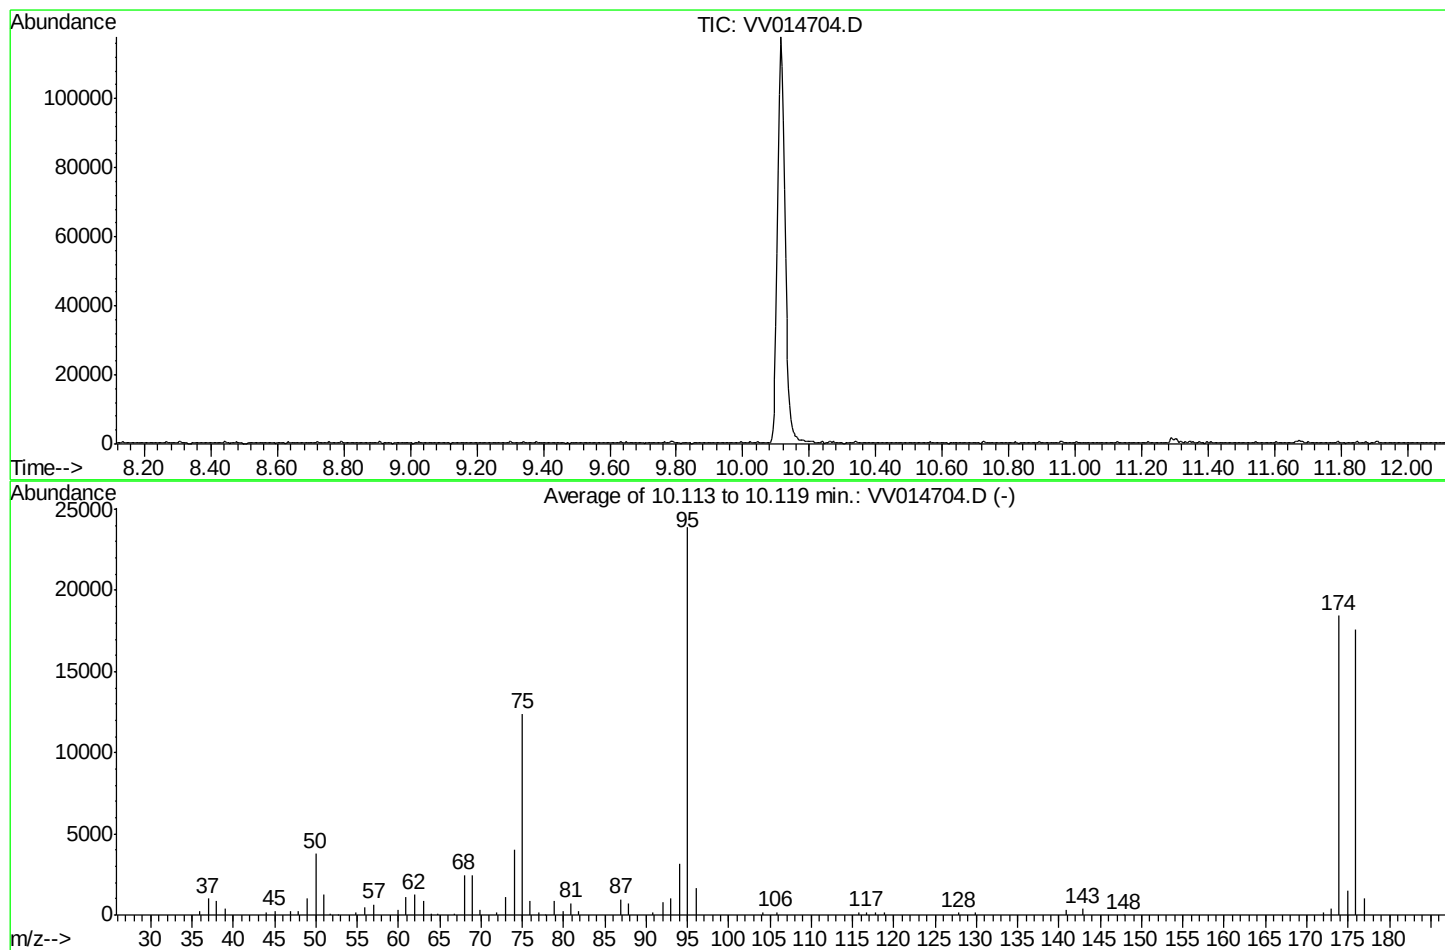

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	3765	PASS
75	95	30	80	52.0	12419	PASS
95	95	100	100	100.0	23890	PASS
96	95	5	9	7.1	1698	PASS
173	174	0.00	2	1.9	358	PASS
174	95	50	120	77.2	18450	PASS
175	174	5	9	8.2	1510	PASS
176	174	95	101	95.3	17581	PASS
177	176	5	9	6.0	1052	PASS

m/z	Abundance
35.90	254.0
37.00	995.0
38.00	951.0
39.00	432.0
40.10	156.0
44.00	365.0
45.00	226.0
46.90	205.0
47.90	219.0
48.90	1072.0
50.00	3794.0
51.00	1310.0
51.80	151.0
52.60	105.0
54.80	119.0
56.00	479.0
57.10	701.0
60.00	231.0
61.00	1077.0
62.00	1289.0
63.00	834.0
64.70	131.0
66.80	110.0
68.00	2338.0
69.00	2456.0
69.90	300.0
72.00	123.0
72.90	1115.0
74.00	4146.0
75.00	12526.0
76.00	945.0
77.00	147.0
78.90	838.0
79.90	243.0
80.90	731.0
81.80	230.0
87.00	1031.0
87.90	816.0
90.80	184.0
92.00	823.0
93.00	972.0
94.00	3342.0
95.00	24336.0
96.00	1644.0
104.00	124.0
105.80	147.0
115.80	151.0
116.70	190.0
117.80	153.0
118.90	125.0
127.90	137.0
129.80	123.0
140.80	332.0
142.90	408.0
147.90	119.0
172.00	184.0
172.90	354.0
173.90	18360.0
174.90	1511.0
175.90	17480.0
176.90	1074.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96

m/z	Abundance
35.90	262.0
37.00	1000.0
38.00	943.0
39.00	415.0
40.00	144.0
43.90	271.0
45.00	239.0
46.90	213.0
47.90	238.0
48.90	1025.0
50.00	3870.0
51.00	1240.0
51.80	144.0
54.90	131.0
55.90	475.0
57.00	681.0
60.00	299.0
61.00	1104.0
62.00	1304.0
63.00	888.0
64.00	104.0
64.80	134.0
66.80	102.0
68.00	2607.0
69.00	2449.0
69.90	323.0
71.90	145.0
72.90	1100.0
74.00	4218.0
75.00	12828.0
76.00	834.0
76.90	181.0
78.90	883.0
79.90	229.0
80.90	729.0
81.80	277.0
86.90	1015.0
87.90	758.0
90.80	178.0
92.00	811.0
93.00	1007.0
94.00	3250.0
95.00	24656.0
96.00	1770.0
104.10	136.0
105.80	184.0
115.80	150.0
116.70	182.0
117.80	143.0
118.80	164.0
127.90	152.0
129.80	134.0
140.80	303.0
142.90	402.0
172.00	197.0
173.00	375.0
173.90	19152.0
174.90	1563.0
175.90	18072.0
176.90	1052.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96

m/z	Abundance
35.90	230.0
36.90	999.0
38.00	824.0
39.00	351.0
39.90	131.0
43.90	230.0
45.00	260.0
46.90	207.0
47.80	218.0
48.90	916.0
50.00	3631.0
51.00	1150.0
55.00	127.0
55.90	417.0
57.00	633.0
60.00	351.0
60.90	1058.0
61.90	1145.0
63.00	794.0
64.00	132.0
68.00	2517.0
69.00	2363.0
69.90	276.0
71.90	163.0
72.90	993.0
74.00	3818.0
75.00	11904.0
75.90	758.0
77.00	180.0
77.80	125.0
78.90	806.0
79.90	192.0
80.90	742.0
81.80	263.0
86.90	888.0
87.90	636.0
90.90	172.0
92.00	748.0
93.00	1009.0
94.00	2881.0
95.00	22680.0
96.00	1681.0
104.10	136.0
105.80	206.0
115.70	140.0
116.80	153.0
117.80	125.0
118.80	177.0
127.90	141.0
129.90	113.0
140.90	286.0
142.90	348.0
172.00	193.0
173.00	345.0
173.90	17840.0
174.90	1456.0
175.90	17192.0
176.90	1030.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96

Scan 2795 (10.077 min): VV014704.D
BFB96

m/z	Abundance
39.90	198.0
44.00	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96