
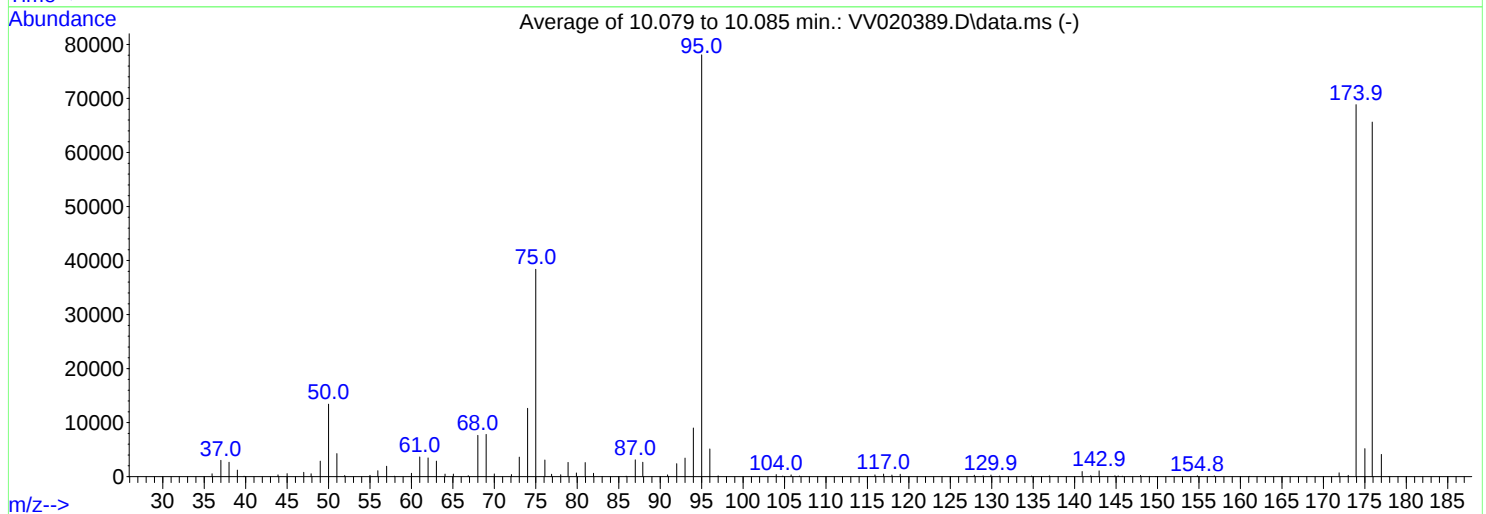


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022521\
 Data File : VV020389.D
 Acq On : 24 Feb 2021 09:09
 Operator : SY/MD
 Sample : BFB86
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB802

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022421WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Feb 25 01:53:18 2021

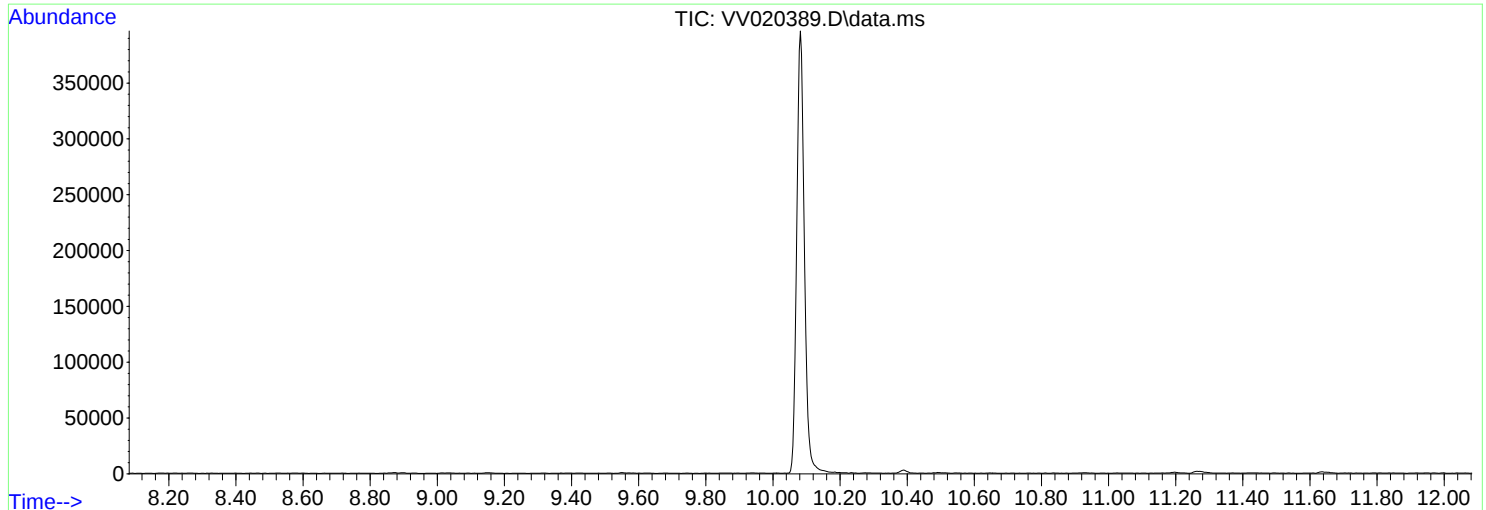

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	13428	PASS
75	95	30	80	49.2	38387	PASS
95	95	100	100	100.0	78072	PASS
96	95	5	9	6.6	5138	PASS
173	174	0.00	2	0.3	235	PASS
174	95	50	120	88.2	68853	PASS
175	174	5	9	7.5	5198	PASS
176	174	95	105	95.3	65616	PASS
177	176	5	10	6.3	4104	PASS

m/z	Abundance
36.00	515.0
37.00	2946.0
38.00	2777.0
39.00	1296.0
39.80	245.0
43.90	851.0
45.00	571.0
47.00	755.0
47.90	466.0
49.00	3014.0
50.00	13655.0
51.00	4159.0
51.90	184.0
55.00	194.0
55.90	1069.0
57.00	1933.0
57.90	155.0
60.00	605.0
61.00	3546.0
62.00	3549.0
63.00	2844.0
64.00	481.0
65.10	487.0
66.80	175.0
68.00	7505.0
69.00	8039.0
70.00	501.0
72.00	402.0
73.00	3524.0
74.00	12741.0
75.00	38408.0
76.10	3129.0
76.90	371.0
78.00	346.0
78.90	2485.0
79.90	666.0
80.90	2588.0
81.90	667.0
83.00	104.0
85.90	111.0
87.00	3177.0
87.90	2714.0
90.90	361.0
92.00	2306.0
93.00	3476.0
94.00	8928.0
95.00	77640.0
96.00	5315.0
97.00	116.0
104.00	413.0
104.80	107.0
105.80	319.0
106.80	106.0
115.90	286.0
117.00	496.0
117.90	309.0
118.90	413.0
127.90	229.0
128.90	128.0
129.90	233.0
131.00	124.0
134.80	198.0
137.00	136.0
140.90	962.0
141.90	146.0
143.00	1111.0
144.90	184.0
145.20	175.0
148.00	215.0
154.80	221.0
156.80	152.0
171.90	637.0
173.00	705.0
173.90	66944.0
175.00	5063.0
175.90	63056.0
177.00	3860.0
177.90	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB802

m/z	Abundance
36.00	536.0
37.00	3151.0
38.00	2746.0
39.00	1236.0
39.80	257.0
44.00	825.0
45.00	578.0
47.00	797.0
47.90	576.0
49.00	2942.0
50.00	13957.0
51.00	4382.0
52.00	219.0
55.00	250.0
56.00	1165.0
57.00	1970.0
58.00	104.0
60.00	652.0
61.00	3788.0
62.00	3553.0
63.00	2990.0
64.10	519.0
65.10	479.0
66.80	198.0
68.00	7902.0
69.00	8098.0
70.00	497.0
72.00	401.0
73.00	3731.0
74.00	13068.0
75.00	39608.0
76.10	3127.0
76.90	482.0
78.00	367.0
78.90	2728.0
79.90	714.0
81.00	2725.0
82.00	669.0
85.90	117.0
87.00	3214.0
87.90	2758.0
90.90	326.0
92.00	2485.0
93.00	3557.0
94.00	9184.0
95.00	80912.0
96.00	5319.0
97.00	158.0
104.00	410.0
104.80	112.0
105.80	330.0
106.80	121.0
115.90	332.0
117.00	481.0
118.00	289.0
119.00	436.0
127.90	281.0
128.90	161.0
129.90	306.0
130.90	110.0
134.80	162.0
137.00	153.0
140.90	993.0
141.90	173.0
143.00	1128.0
144.80	189.0
145.30	164.0
145.70	125.0
147.90	220.0
149.00	104.0
149.80	100.0
154.80	174.0
156.80	160.0
161.10	105.0
171.90	715.0
174.00	70992.0
175.00	5372.0
175.90	67960.0
177.00	4250.0

Instrument :
MSVOA_V
ClientSampleId :
BFB802

m/z	Abundance
35.90	568.0
37.00	2935.0
38.00	2461.0
39.00	1129.0
39.80	258.0
43.90	749.0
45.00	519.0
47.00	867.0
47.90	596.0
49.00	2658.0
50.00	12673.0
51.00	4221.0
52.00	260.0
55.00	254.0
56.00	1064.0
57.00	1893.0
60.00	590.0
61.00	3643.0
62.00	3273.0
63.00	2820.0
64.10	473.0
65.00	443.0
66.90	203.0
68.00	7547.0
69.00	7351.0
70.00	511.0
72.10	372.0
73.00	3561.0
74.00	12114.0
75.00	37144.0
76.10	3010.0
76.90	483.0
78.00	345.0
78.90	2698.0
79.90	714.0
81.00	2542.0
82.00	578.0
87.00	2978.0
87.90	2531.0
90.90	295.0
92.00	2374.0
93.00	3319.0
94.00	8881.0
95.00	75664.0
96.00	4781.0
97.00	177.0
104.00	334.0
104.80	105.0
105.80	299.0
106.80	125.0
115.90	327.0
116.80	421.0
117.90	265.0
119.00	451.0
127.90	314.0
129.00	164.0
129.90	330.0
130.90	103.0
135.00	126.0
136.90	158.0
140.90	901.0
142.00	192.0
142.90	971.0
144.80	159.0
145.30	132.0
145.80	150.0
147.90	202.0
149.00	119.0
154.80	156.0
156.90	156.0
161.00	108.0
171.90	749.0
174.00	68624.0
175.00	5158.0
175.90	65832.0
177.00	4203.0

Instrument :
MSVOA_V
ClientSampleId :
BFB802

m/z	Abundance
39.90	162.0
43.90	480.0

Instrument :
MSVOA_V
ClientSampleId :
BFB802