

Data File : VV009377.D
Acq On : 26 Feb 2019 19:56
Operator : SY/MD
Sample : K1601-08
Misc : 4.89G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF7Y2RE

Quant Time: Feb 27 04:48:29 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM022619S.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 27 04:43:55 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	129912	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	107917	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	38120	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	43584	26.67	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	106.68%
7) Chloroethane-d5	1.58	69	62740	29.52	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	118.08%
10) 1,1-Dichloroethene-d2	2.13	63	87055	20.14	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	80.56%
20) 2-Butanone-d5	3.95	46	21369	43.40	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.80%
24) Chloroform-d	4.40	84	79536	25.24	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	100.96%
26) 1,2-Dichloroethane-d4	5.08	65	48733	27.96	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	111.84%
29) Benzene-d6	5.10	84	165090	28.78	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	115.12%
33) 1,2-Dichloropropane-d6	6.12	67	51963	30.91	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	123.64%#
37) Toluene-d8	7.36	98	141866	25.78	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	103.12%
38) trans-1,3-Dichloropropene-	7.67	79	20572	24.48	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.92%
39) 2-Hexanone-d5	8.14	63	17727	49.82	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.64%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	42850	26.10	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	104.40%
61) 1,2-Dichlorobenzene-d4	11.68	152	33532	23.75	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.00%

Target Compounds


					Qvalue
13) Acetone	2.21	43	1589	2.823 ug/L	79
16) Methylene chloride	2.54	84	4880	2.773 ug/L	98
35) Trichloroethene	5.66	95	3998	2.400 ug/L #	6
40) 1,2-Dichloropropane	6.12	63	5832	3.902 ug/L #	89
42) cis-1,3-Dichloropropene	7.03	75	1370	0.577 ug/L #	70
45) trans-1,3-Dichloropropene	7.66	75	1009	0.469 ug/L #	78
49) 2-Hexanone	8.18	43	3767	4.222 ug/L #	45
59) 1,2,3-Trichloropropane	11.30	75	5419	4.532 ug/L #	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV009377.D
Acq On : 26 Feb 2019 19:56
Operator : SY/MD
Sample : K1601-08
Misc : 4.89G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF7Y2RE

Quant Time: Feb 27 04:48:29 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM022619S.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 27 04:43:55 2019
Response via : Initial Calibration

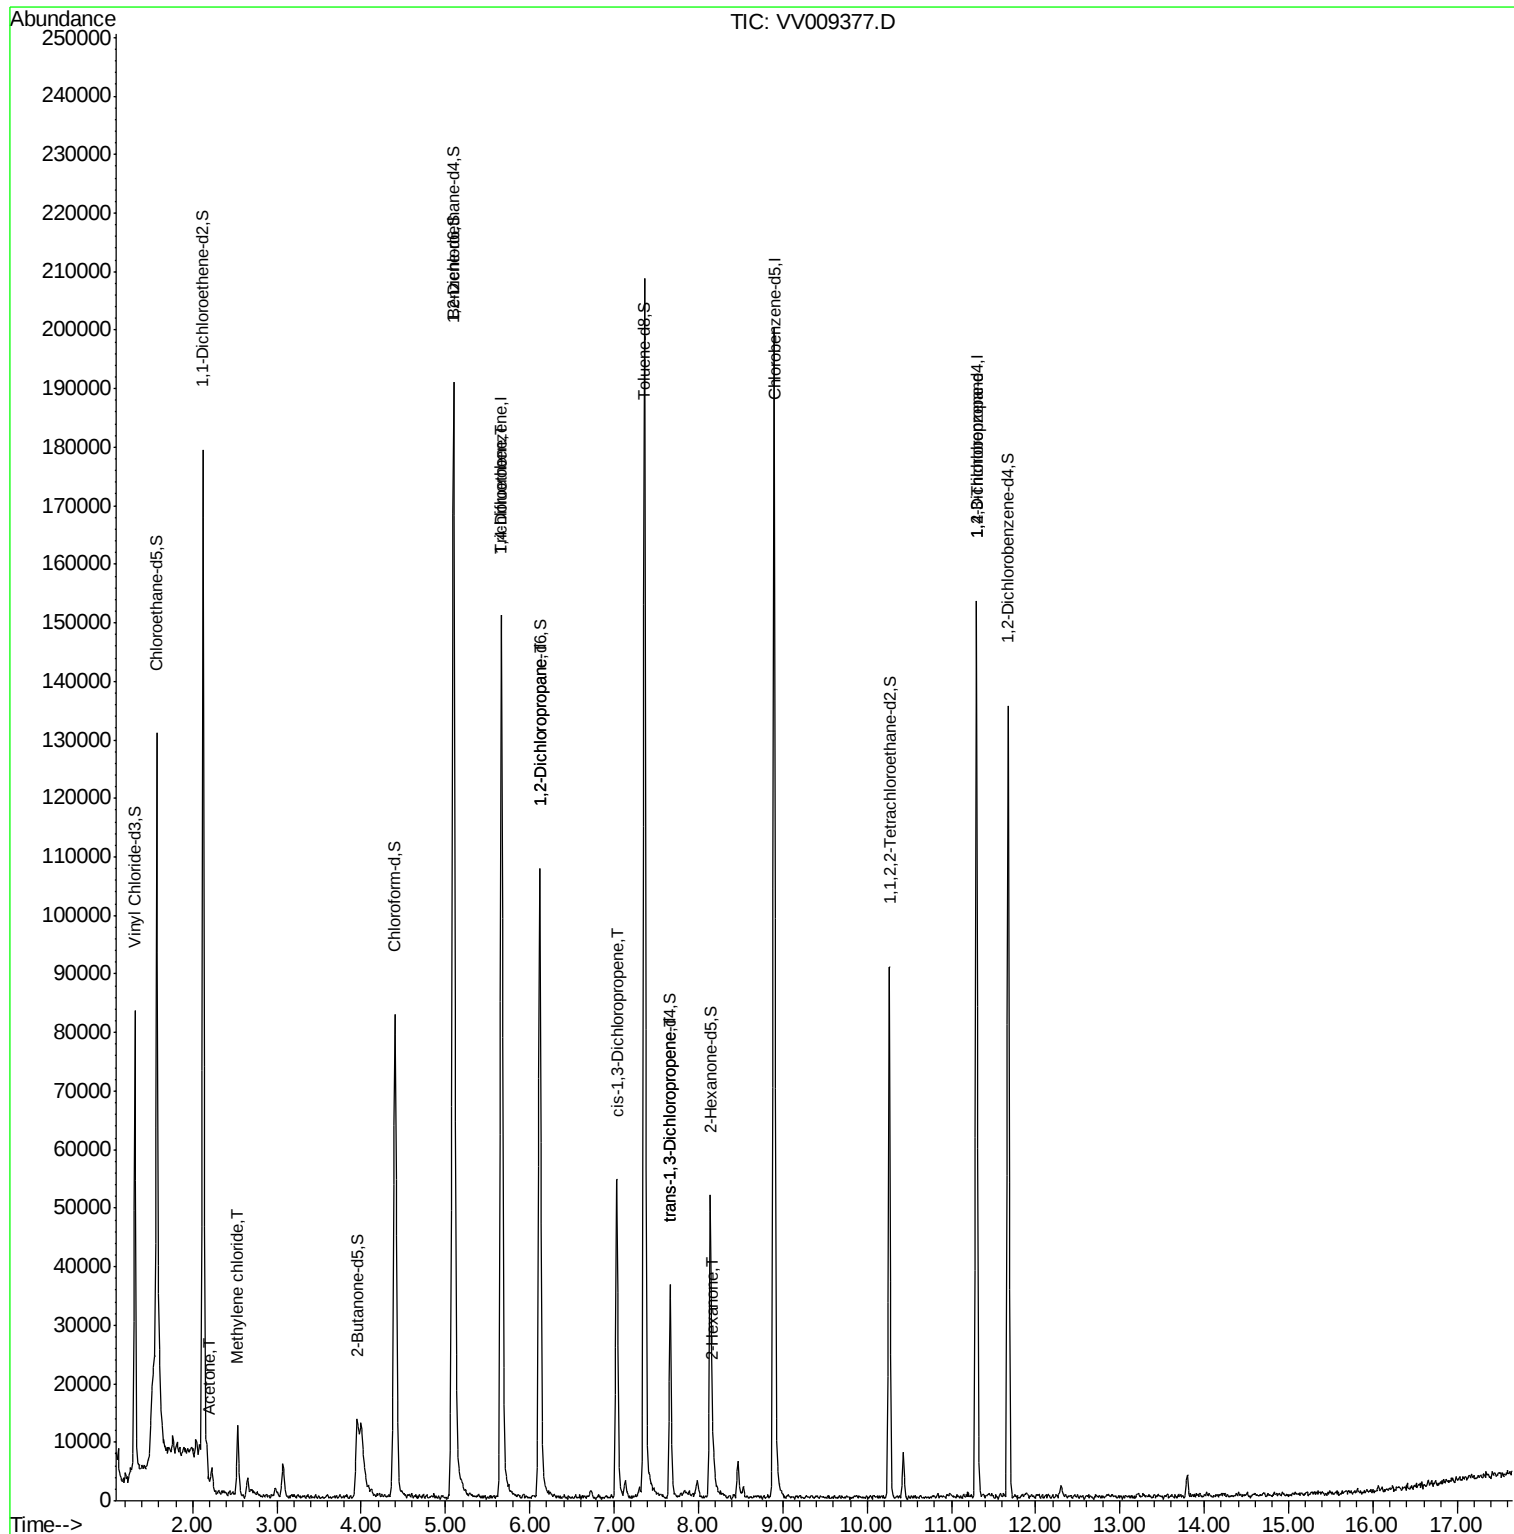

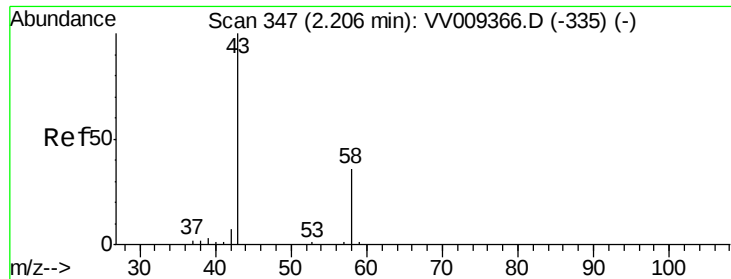

#13

Acetone

Concen: 2.823 ug/L

RT: 2.21 min Scan# 347

Delta R.T. 0.00 min

Lab File: VV009377.D

Acq: 26 Feb 2019 19:56

Instrument :

MSVOA_V

ClientSampleId :


BF7Y2RE

Tgt Ion: 43 Resp: 1589

Ion Ratio Lower Upper




43 100

58 22.5 0.0 68.8

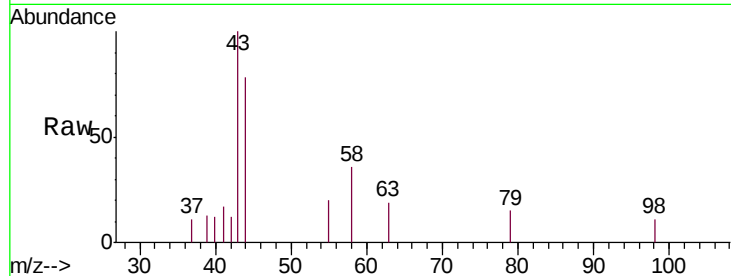

Abundance Ion 43.00 (42.70 to 43.70): VV009366.D (-335) (-)

Ion 58.00 (57.70 to 58.70): VV009366.D (-335) (-)

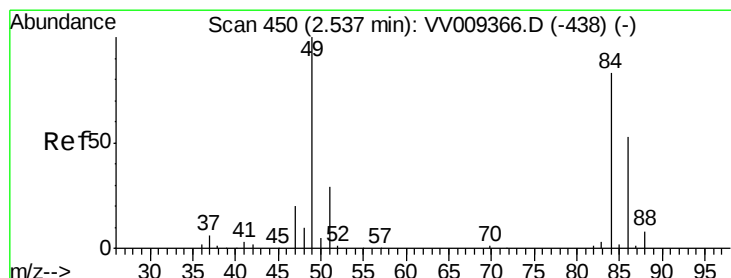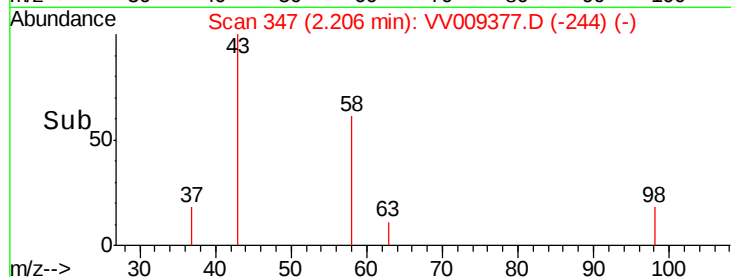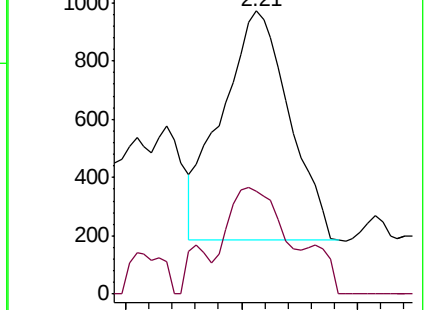

#16

Methylene chloride

Concen: 2.773 ug/L

RT: 2.54 min Scan# 450

Delta R.T. 0.00 min

Lab File: VV009377.D

Acq: 26 Feb 2019 19:56


Tgt Ion: 84 Resp: 4880

Ion Ratio Lower Upper

84 100

49 118.7 84.6 157.0



86 68.1 46.1 85.7

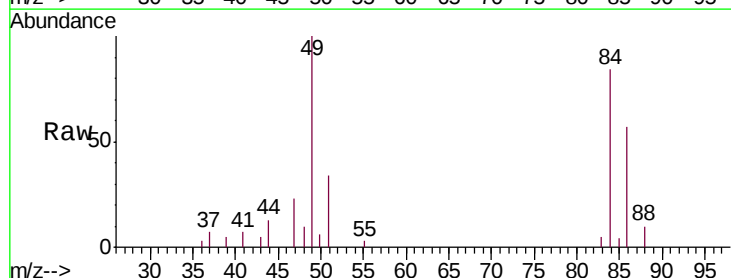


Abundance Ion 84.00 (83.70 to 84.70): VV009366.D (-438) (-)

Ion 49.00 (48.70 to 49.70): VV009366.D (-438) (-)

Ion 86.00 (85.70 to 86.70): VV009366.D (-438) (-)

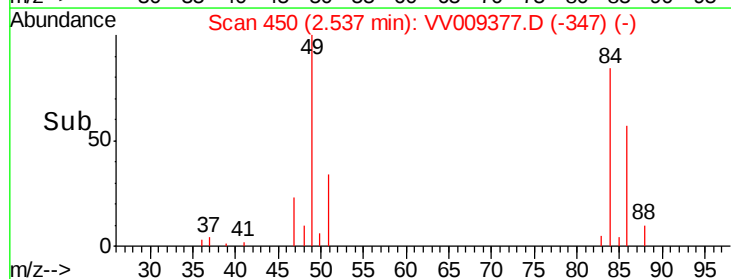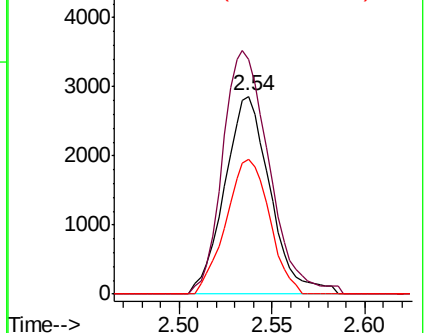

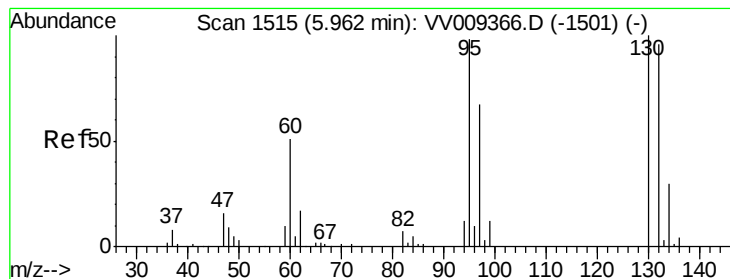

#35

Trichloroethene

Concen: 2.400 ug/L

RT: 5.66 min Scan# 1422

Delta R.T. -0.30 min

Lab File: VV009377.D

Acq: 26 Feb 2019 19:56

Instrument :

MSVOA_V

ClientSampleId :

BF7Y2RE

Tgt Ion: 95 Resp: 3998





Ion Ratio Lower Upper

95 100

97 0.0 44.3 82.3#

132 0.0 64.4 119.6#

130 0.0 69.4 128.8#

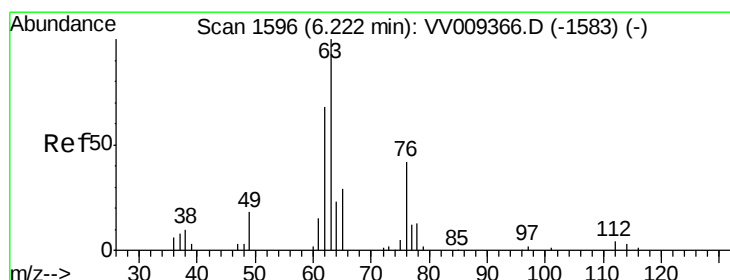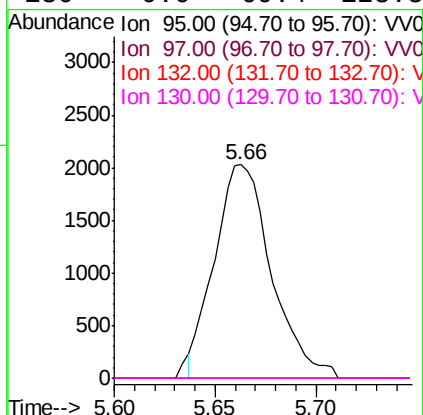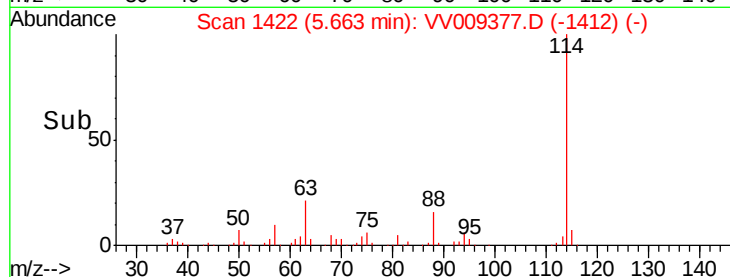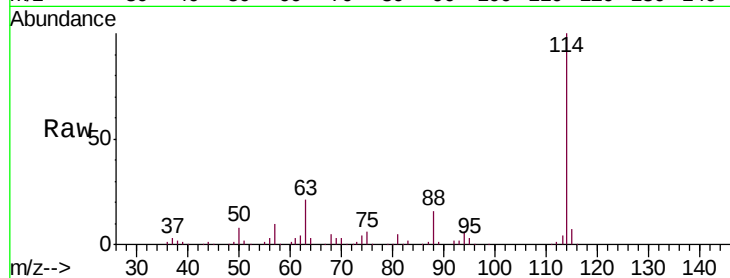

#40

1,2-Dichloropropane

Concen: 3.902 ug/L

RT: 6.12 min Scan# 1564

Delta R.T. -0.10 min

Lab File: VV009377.D




Acq: 26 Feb 2019 19:56


Tgt Ion: 63 Resp: 5832

Ion Ratio Lower Upper

63 100

112 0.0 3.0 4.4#

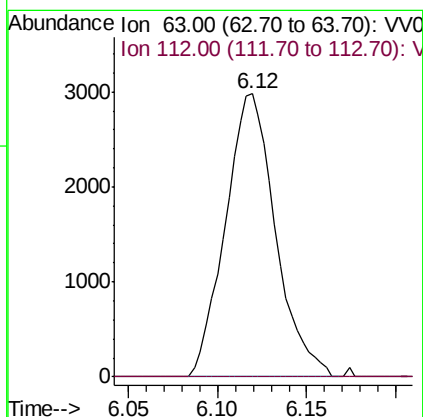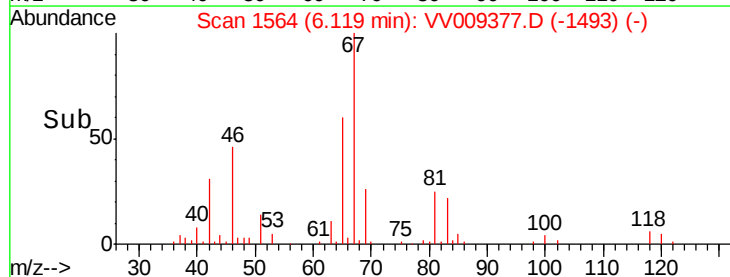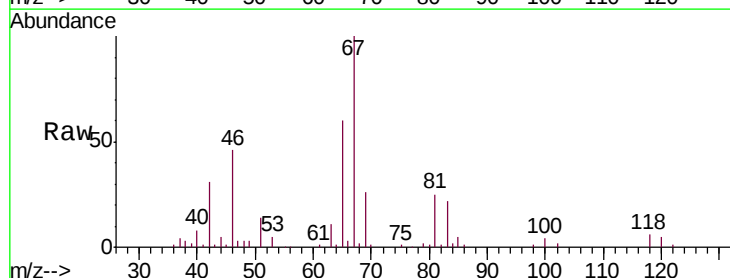

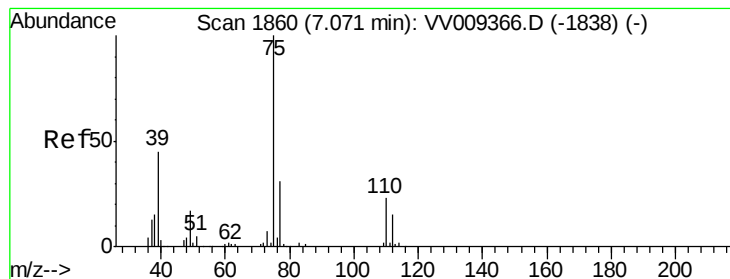

#42

cis-1,3-Dichloropropene

Concen: 0.577 ug/L

RT: 7.03 min Scan# 1848

Delta R.T. -0.04 min

Lab File: VV009377.D

Acq: 26 Feb 2019 19:56

Instrument :

MSVOA_V

ClientSampleId :


BF7Y2RE

Tgt Ion: 75 Resp: 1370

Ion Ratio Lower Upper

75 100

77 47.0 21.4 39.8#

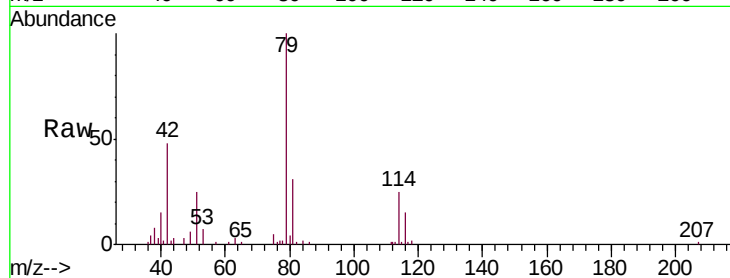

Abundance Ion 75.00 (74.70 to 75.70): VV0

Ion 77.00 (76.70 to 77.70): VV0

7.03

800

600



400

200

0

7.00 7.02 7.04 7.06

Time-->

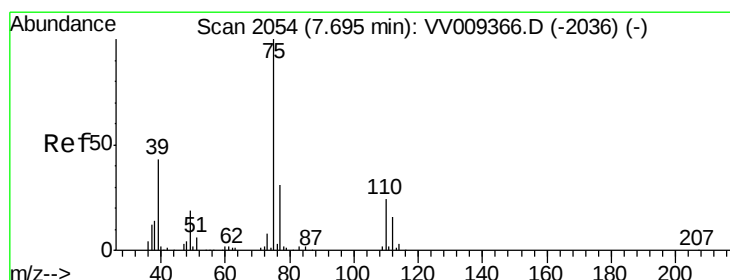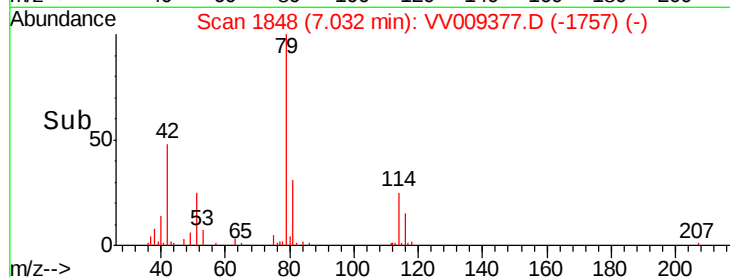

#45

trans-1,3-Dichloropropene

Concen: 0.469 ug/L

RT: 7.66 min Scan# 2044

Delta R.T. -0.03 min

Lab File: VV009377.D


Acq: 26 Feb 2019 19:56

Tgt Ion: 75 Resp: 1009

Ion Ratio Lower Upper

75 100

77 44.3 22.5 41.7#

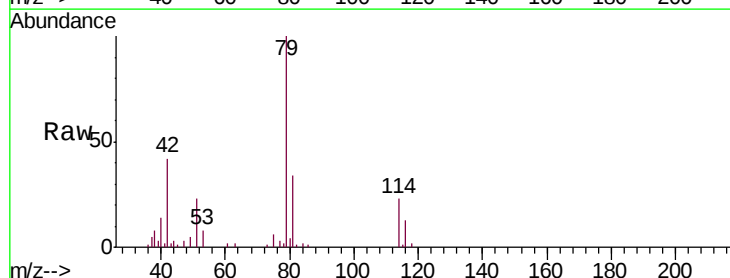

Abundance Ion 75.00 (74.70 to 75.70): VV0

Ion 77.00 (76.70 to 77.70): VV0

7.66

800

600


400


200

0

7.64 7.66 7.68 7.70

Time-->




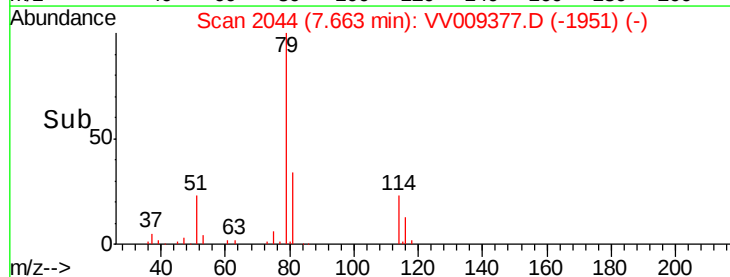


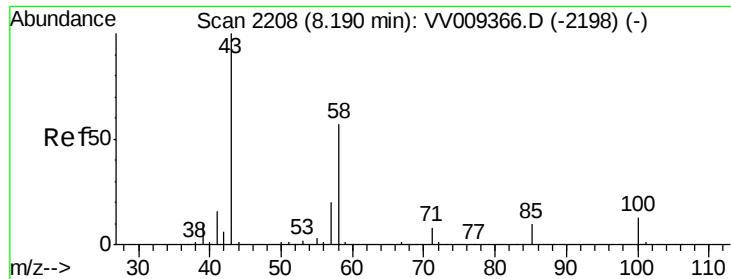

#49
2-Hexanone
Concen: 4.222 ug/L
RT: 8.18 min Scan# 2204
Delta R.T. -0.01 min
Lab File: VV009377.D
Acq: 26 Feb 2019 19:56

Instrument :
MSVOA_V
ClientSampleId :
BF7Y2RE

Tgt Ion: 43 Resp: 3767
Ion Ratio Lower Upper
43 100
58 9.9 46.3 69.5#
57 1.8 15.8 23.6#
100 0.0 10.0 15.0#

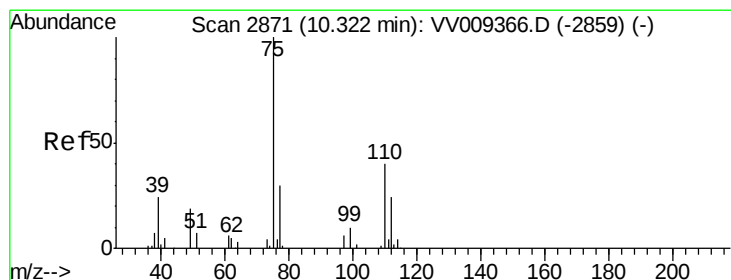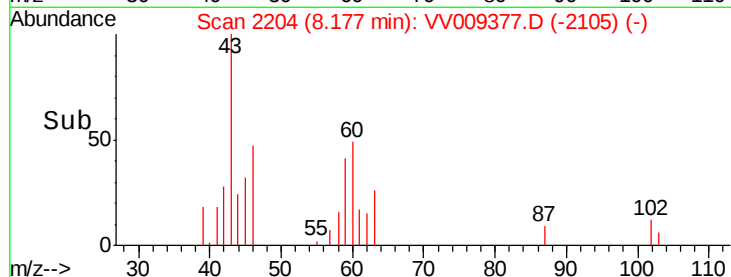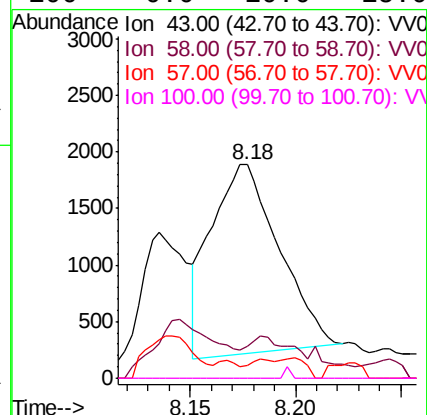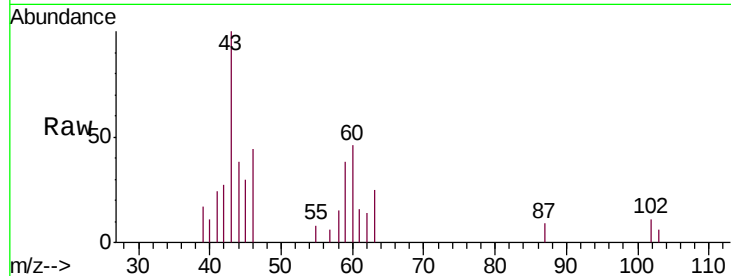

#59
1,2,3-Trichloropropane
Concen: 4.532 ug/L
RT: 11.30 min Scan# 3174
Delta R.T. 0.97 min
Lab File: VV009377.D
Acq: 26 Feb 2019 19:56

Tgt Ion: 75 Resp: 5419
Ion Ratio Lower Upper
75 100
77 40.7 25.9 38.9#

