

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022619\
 Data File : VV009380.D
 Acq On : 26 Feb 2019 21:15
 Operator : SY/MD
 Sample : K1622-02
 Misc : 4.88G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BF5H7

Quant Time: Feb 27 06:24:48 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM022619S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Feb 27 04:43:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	138010	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	121814	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	48500	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	33965	19.56	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.24%
7) Chloroethane-d5	1.58	69	58143	25.75	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.00%
10) 1,1-Dichloroethene-d2	2.13	63	72788	15.85	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.40%
20) 2-Butanone-d5	3.96	46	19299	36.89	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	73.78%
24) Chloroform-d	4.40	84	78202	23.36	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.44%
26) 1,2-Dichloroethane-d4	5.08	65	46363	25.04	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.16%
29) Benzene-d6	5.10	84	157697	24.35	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.40%
33) 1,2-Dichloropropane-d6	6.12	67	50834	26.79	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	107.16%
37) Toluene-d8	7.36	98	145080	23.36	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.44%
38) trans-1,3-Dichloropropene-	7.67	79	20588	21.70	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.80%
39) 2-Hexanone-d5	8.14	63	17608	43.84	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.68%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	44866	24.21	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.84%
61) 1,2-Dichlorobenzene-d4	11.67	152	42004	23.38	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.52%


Target Compounds					Ovalue
13) Acetone	2.21	43	2214	3.702 ug/L	98
16) Methylene chloride	2.53	84	4774	2.554 ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV022619\
Data File : VV009380.D
Acq On : 26 Feb 2019 21:15
Operator : SY/MD
Sample : K1622-02
Misc : 4.88G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF5H7

Quant Time: Feb 27 06:24:48 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM022619S.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 27 04:43:55 2019
Response via : Initial Calibration

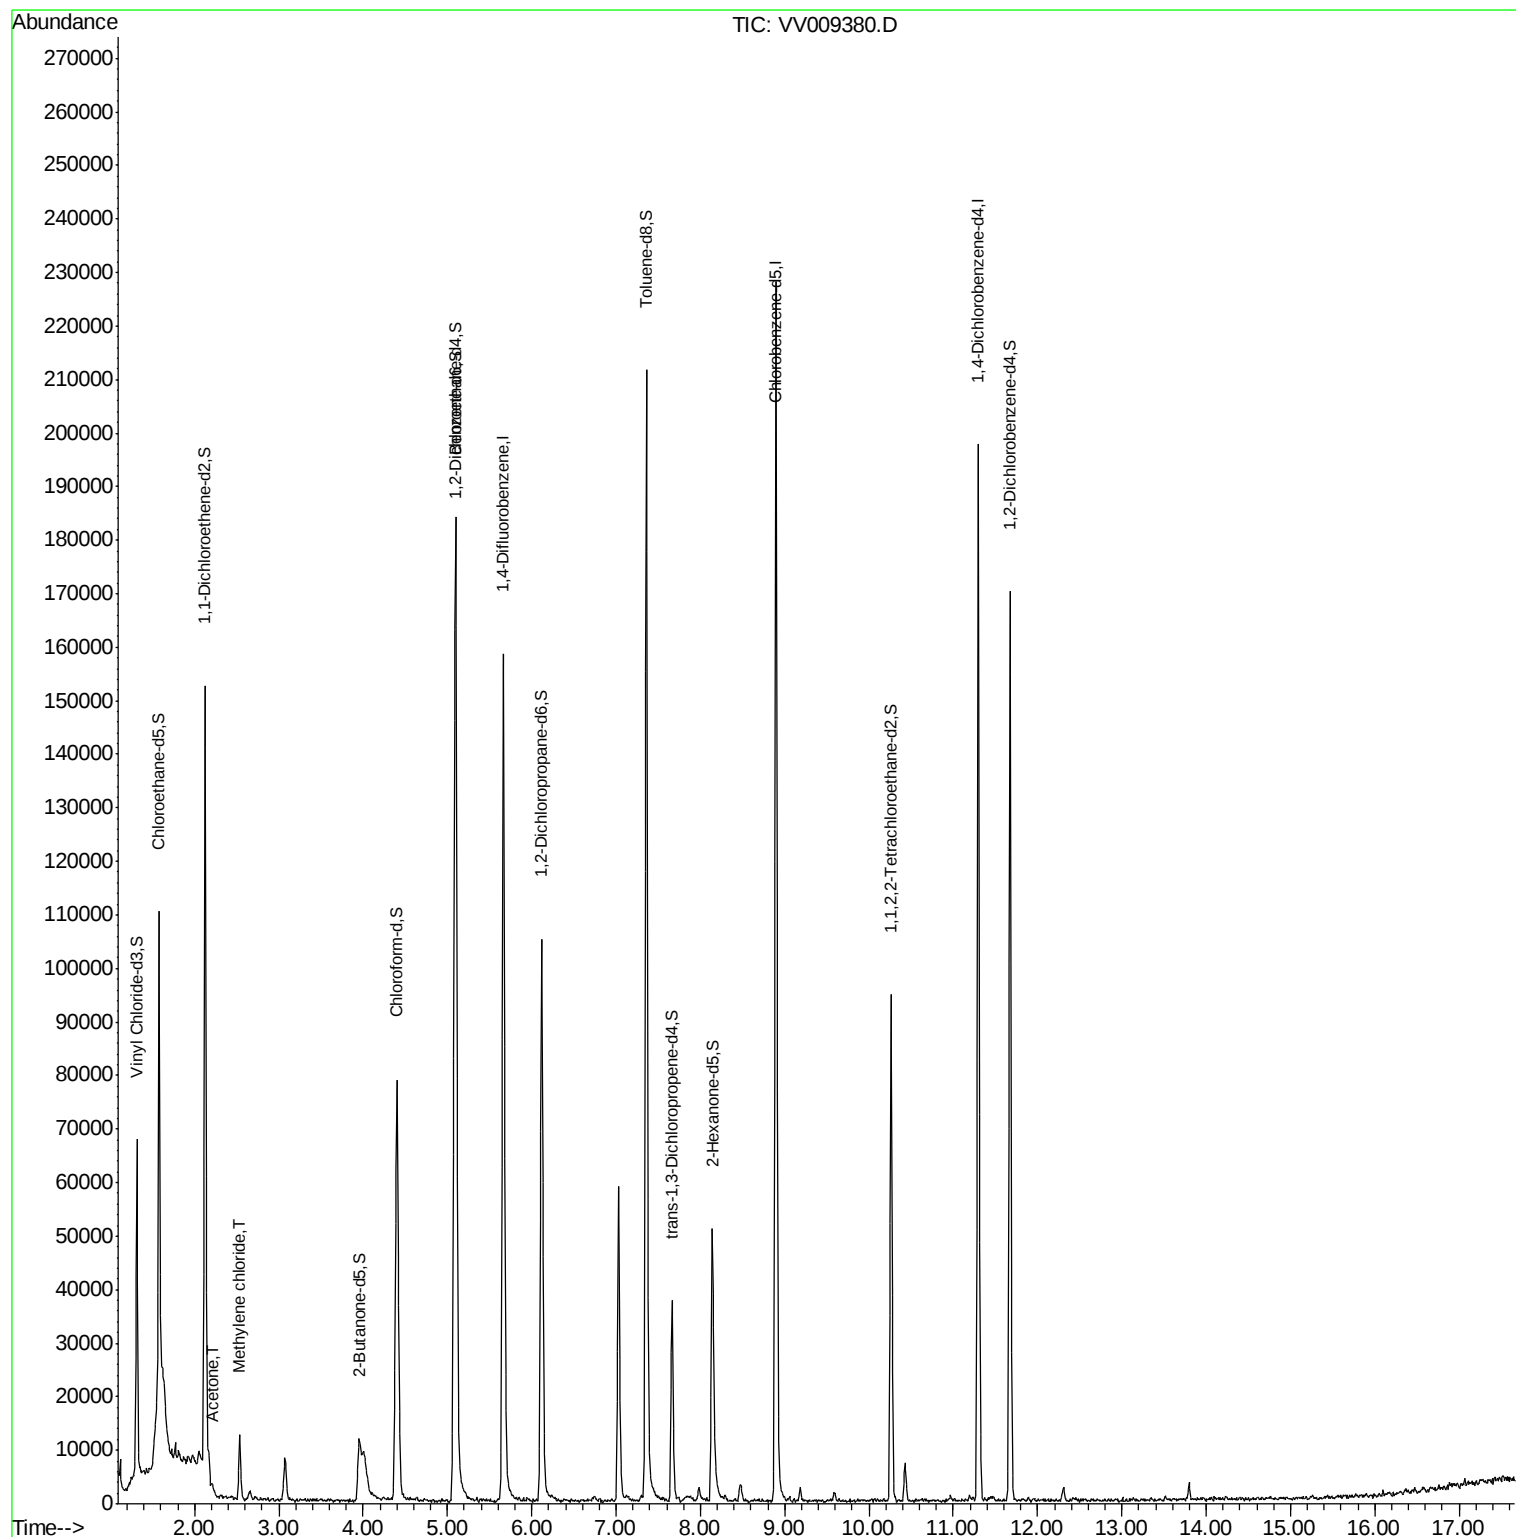

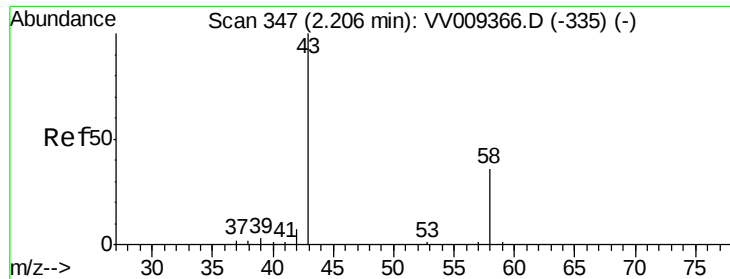

#13

Acetone

Concen: 3.702 ug/L

RT: 2.21 min Scan# 347

Delta R.T. -0.00 min

Lab File: VV009380.D

Acq: 26 Feb 2019 21:15

Instrument :

MSVOA_V

ClientSampled :


BF5H7

Tot Ion: 43 Resp: 2214

Ion Ratio Lower Upper




43 100

58 33.5 0.0 68.8

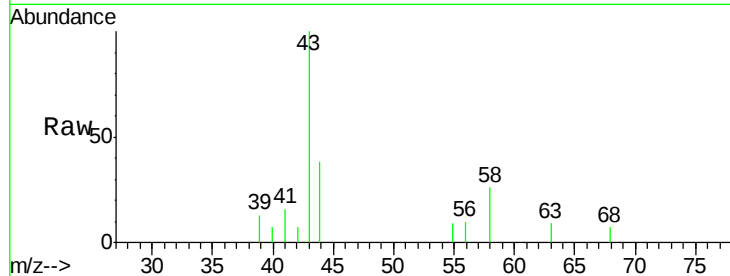

Abundance Ion 43.00 (42.70 to 43.70): VV009380.D (-244) (-)

Ion 58.00 (57.70 to 58.70): VV009380.D (-244) (-)

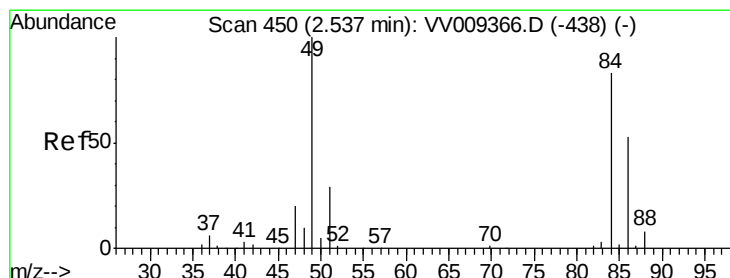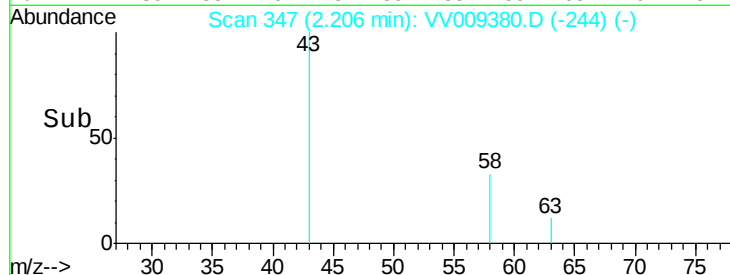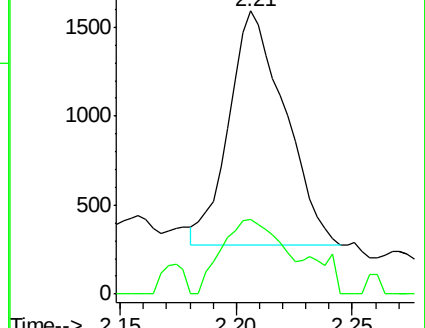

#16

Methylene chloride

Concen: 2.554 ug/L

RT: 2.53 min Scan# 449

Delta R.T. -0.00 min

Lab File: VV009380.D

Acq: 26 Feb 2019 21:15


Tgt Ion: 84 Resp: 4774

Ion Ratio Lower Upper

84 100

49 138.1 84.6 157.0

86 70.2 46.1 85.7

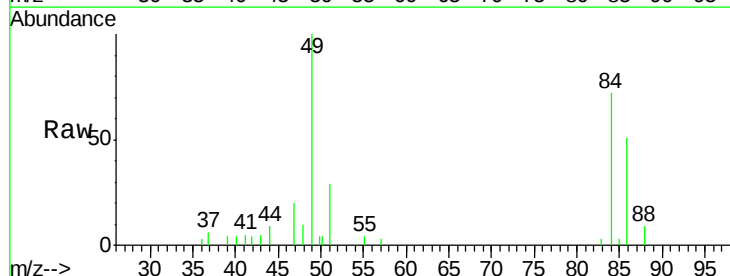

Abundance Ion 84.00 (83.70 to 84.70): VV009380.D (-347) (-)

Ion 49.00 (48.70 to 49.70): VV009380.D (-347) (-)

Ion 86.00 (85.70 to 86.70): VV009380.D (-347) (-)

