


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022619\
 Data File : VV009359.D
 Acq On : 26 Feb 2019 09:25
 Operator : SY/MD
 Sample : BFB67
 Misc : 5.00G/10ML/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB67

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM022619S.M
 Title : VOC Analysis
 Last Update : Thu Feb 28 04:32:57 2019

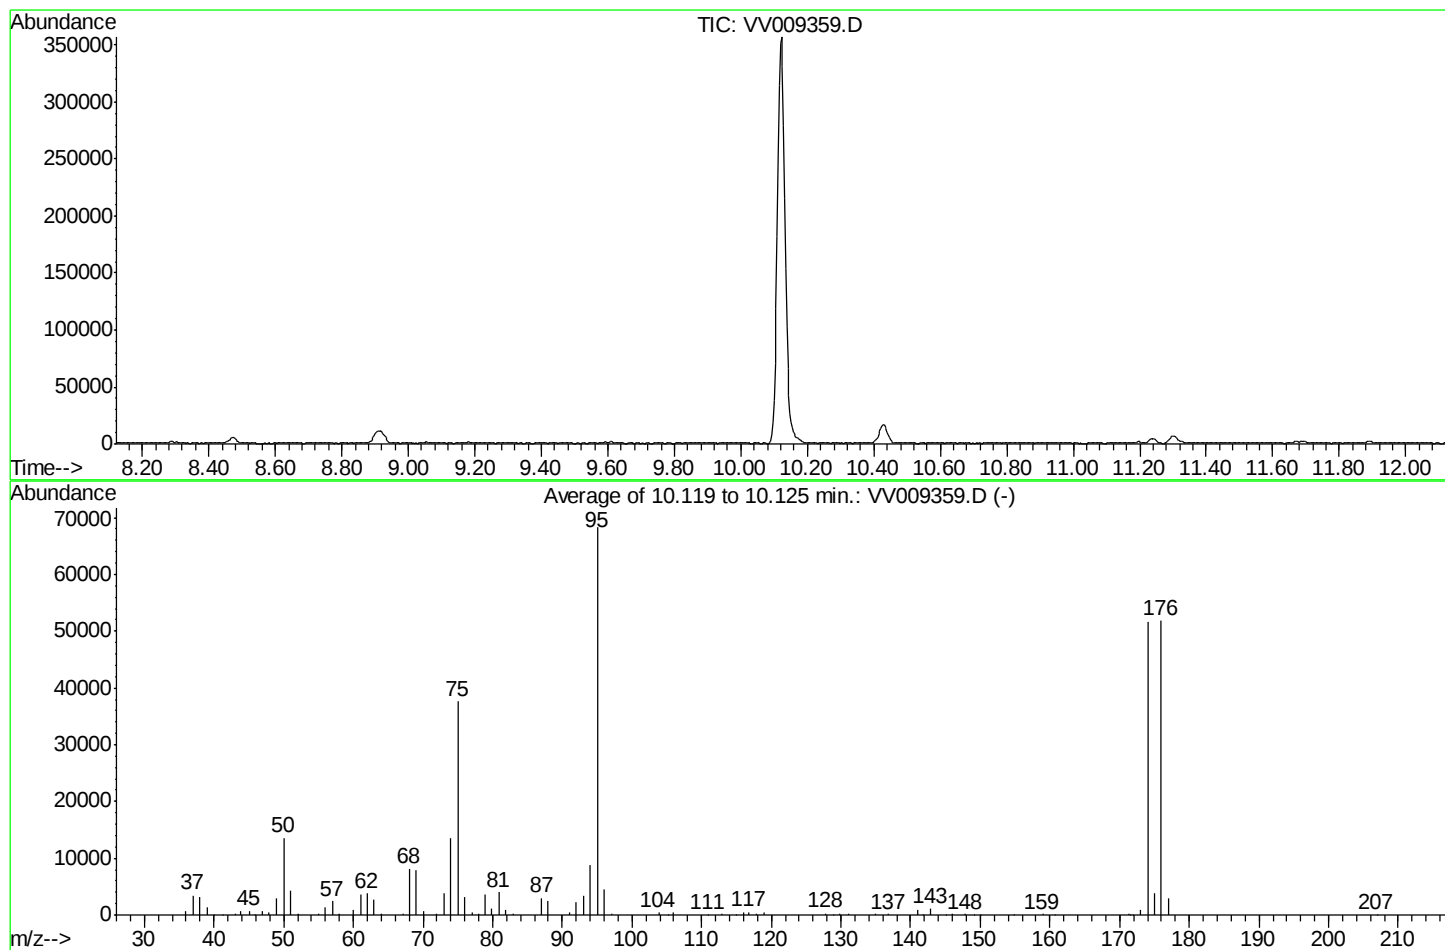

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	13603	PASS
75	95	30	80	55.1	37640	PASS
95	95	100	100	100.0	68296	PASS
96	95	5	9	6.5	4417	PASS
173	174	0.00	2	2.0	1019	PASS
174	95	50	120	75.7	51730	PASS
175	174	5	9	7.5	3854	PASS
176	174	95	101	100.1	51781	PASS
177	176	5	9	5.8	2985	PASS

m/z	Abundance
36.00	610.0
37.00	3582.0
38.00	3374.0
39.00	1348.0
39.90	142.0
43.10	105.0
44.00	959.0
45.00	725.0
45.90	115.0
47.00	689.0
47.90	448.0
49.00	3057.0
50.00	14078.0
51.00	4656.0
52.10	237.0
55.10	297.0
56.00	1531.0
57.10	2572.0
58.00	110.0
59.90	882.0
61.00	3661.0
62.00	3833.0
63.00	2804.0
64.00	379.0
67.10	300.0
68.00	8575.0
69.00	8200.0
70.00	732.0
72.00	341.0
73.00	3959.0
74.00	13848.0
75.00	39160.0
76.00	3460.0
77.00	483.0
77.90	335.0
78.90	3759.0
79.90	1088.0
80.90	4033.0
81.90	942.0
82.90	172.0
87.00	2937.0
87.90	2576.0
91.00	383.0
92.00	2298.0
93.00	3535.0
94.00	9109.0
95.00	68696.0
96.00	4623.0
97.10	131.0
103.90	437.0
105.90	378.0
112.90	137.0
115.00	112.0
115.90	389.0
116.90	611.0
117.80	336.0
118.90	554.0
127.80	306.0
128.80	115.0
129.80	290.0
131.00	139.0
134.80	174.0
136.80	206.0
141.00	984.0
142.90	993.0
145.00	132.0
146.00	133.0
147.90	154.0
159.00	165.0
160.90	110.0
171.60	166.0
173.00	1031.0
174.00	51384.0
175.00	3997.0
176.00	51600.0
177.00	3055.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
36.00	582.0
37.00	3481.0
38.00	3406.0
39.00	1308.0
39.90	107.0
41.20	119.0
43.10	159.0
43.90	962.0
45.00	712.0
45.90	118.0
47.00	748.0
47.90	415.0
49.00	3109.0
50.00	14044.0
51.00	4423.0
52.10	202.0
55.00	221.0
56.00	1482.0
57.00	2517.0
58.00	125.0
60.00	874.0
61.00	3623.0
62.00	3894.0
63.00	2695.0
64.00	325.0
67.10	348.0
68.00	8562.0
69.00	8205.0
70.00	679.0
72.00	333.0
73.00	3852.0
74.00	14101.0
75.00	38688.0
76.00	3297.0
77.00	476.0
77.90	294.0
78.90	3794.0
79.90	1104.0
80.90	4178.0
81.90	930.0
82.90	202.0
87.00	3031.0
87.90	2580.0
91.00	410.0
92.00	2402.0
93.00	3562.0
94.00	9049.0
95.00	70504.0
96.00	4524.0
97.10	162.0
103.90	432.0
105.90	372.0
111.00	104.0
112.90	147.0
114.90	119.0
115.90	402.0
116.90	562.0
117.80	336.0
118.90	538.0
127.80	317.0
128.80	114.0
129.80	295.0
131.00	161.0
134.90	146.0
136.80	234.0
141.00	1045.0
141.70	124.0
142.90	1073.0
145.90	121.0
147.80	189.0
154.80	109.0
159.00	190.0
160.70	111.0
171.30	193.0
173.00	1056.0
174.00	53144.0
175.00	3874.0
176.00	53480.0
177.00	3058.0
206.90	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
36.00	545.0
37.00	3128.0
38.00	2938.0
39.00	1235.0
41.20	104.0
43.10	192.0
43.90	933.0
45.10	669.0
45.90	123.0
47.00	736.0
47.90	378.0
49.00	2939.0
50.00	12688.0
51.00	3948.0
51.90	189.0
54.80	196.0
56.00	1239.0
57.00	2214.0
58.00	161.0
60.00	706.0
61.00	3473.0
62.00	3637.0
63.00	2584.0
64.00	250.0
67.10	348.0
68.00	7497.0
69.00	7434.0
70.00	620.0
71.90	306.0
73.00	3374.0
74.00	12999.0
75.00	35072.0
76.00	3025.0
77.00	391.0
77.90	258.0
78.90	3455.0
79.90	996.0
80.90	3840.0
81.80	820.0
83.00	212.0
87.00	2931.0
87.90	2522.0
91.00	389.0
92.00	2284.0
93.00	3185.0
94.00	8410.0
95.00	65688.0
96.00	4105.0
97.10	163.0
103.90	367.0
105.10	100.0
105.90	388.0
110.90	107.0
112.90	135.0
116.00	355.0
116.80	488.0
117.80	298.0
118.90	521.0
127.90	273.0
128.90	113.0
129.80	247.0
131.00	130.0
135.00	107.0
136.80	205.0
140.90	1013.0
141.70	142.0
142.90	1025.0
145.80	127.0
147.80	210.0
149.10	101.0
150.00	110.0
154.80	166.0
159.00	166.0
160.70	101.0
171.30	170.0
171.80	123.0
173.00	970.0
174.00	50664.0
175.00	3692.0
176.00	50264.0
177.00	2843.0
206.90	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
43.90	290.0
54.90	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67