

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022621\
 Data File : VV020402.D
 Acq On : 24 Feb 2021 19:05
 Operator : SY/MD
 Sample : VV0226WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK167

Quant Time: Feb 25 00:38:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Feb 24 17:44:20 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	588187	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	567269	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	289167	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	143028	49.14	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	98.28%		
7) Chloroethane-d5	1.571	69	130754	50.27	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	100.54%		
11) 1,1-Dichloroethene-d2	2.111	63	215171	35.83	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	71.66%		
21) 2-Butanone-d5	3.892	46	219780	100.30	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	100.30%		
24) Chloroform-d	4.352	84	320618	48.18	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.36%		
26) 1,2-Dichloroethane-d4	5.037	65	215048	51.14	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.28%		
32) Benzene-d6	5.053	84	650444	52.63	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	105.26%		
36) 1,2-Dichloropropane-d6	6.075	67	202482	52.34	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	104.68%		
41) Toluene-d8	7.320	98	601463	51.05	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.10%		
43) trans-1,3-Dichloroprop...	7.625	79	91389	48.97	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	97.94%		
47) 2-Hexanone-d5	8.091	63	145745	95.04	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	95.04%		
56) 1,1,2,2-Tetrachloroeth...	10.223	84	261731	47.71	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	95.42%		
66) 1,2-Dichlorobenzene-d4	11.632	152	272069	53.85	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	107.70%		
Target Compounds					Qvalue	
48) 2-Hexanone	8.153	43	12642	3.65	ug/L #	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022621\
Data File : VV020402.D
Acq On : 24 Feb 2021 19:05
Operator : SY/MD
Sample : VV0226WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK167

Quant Time: Feb 25 00:38:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022621WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 24 17:44:20 2021
Response via : Initial Calibration

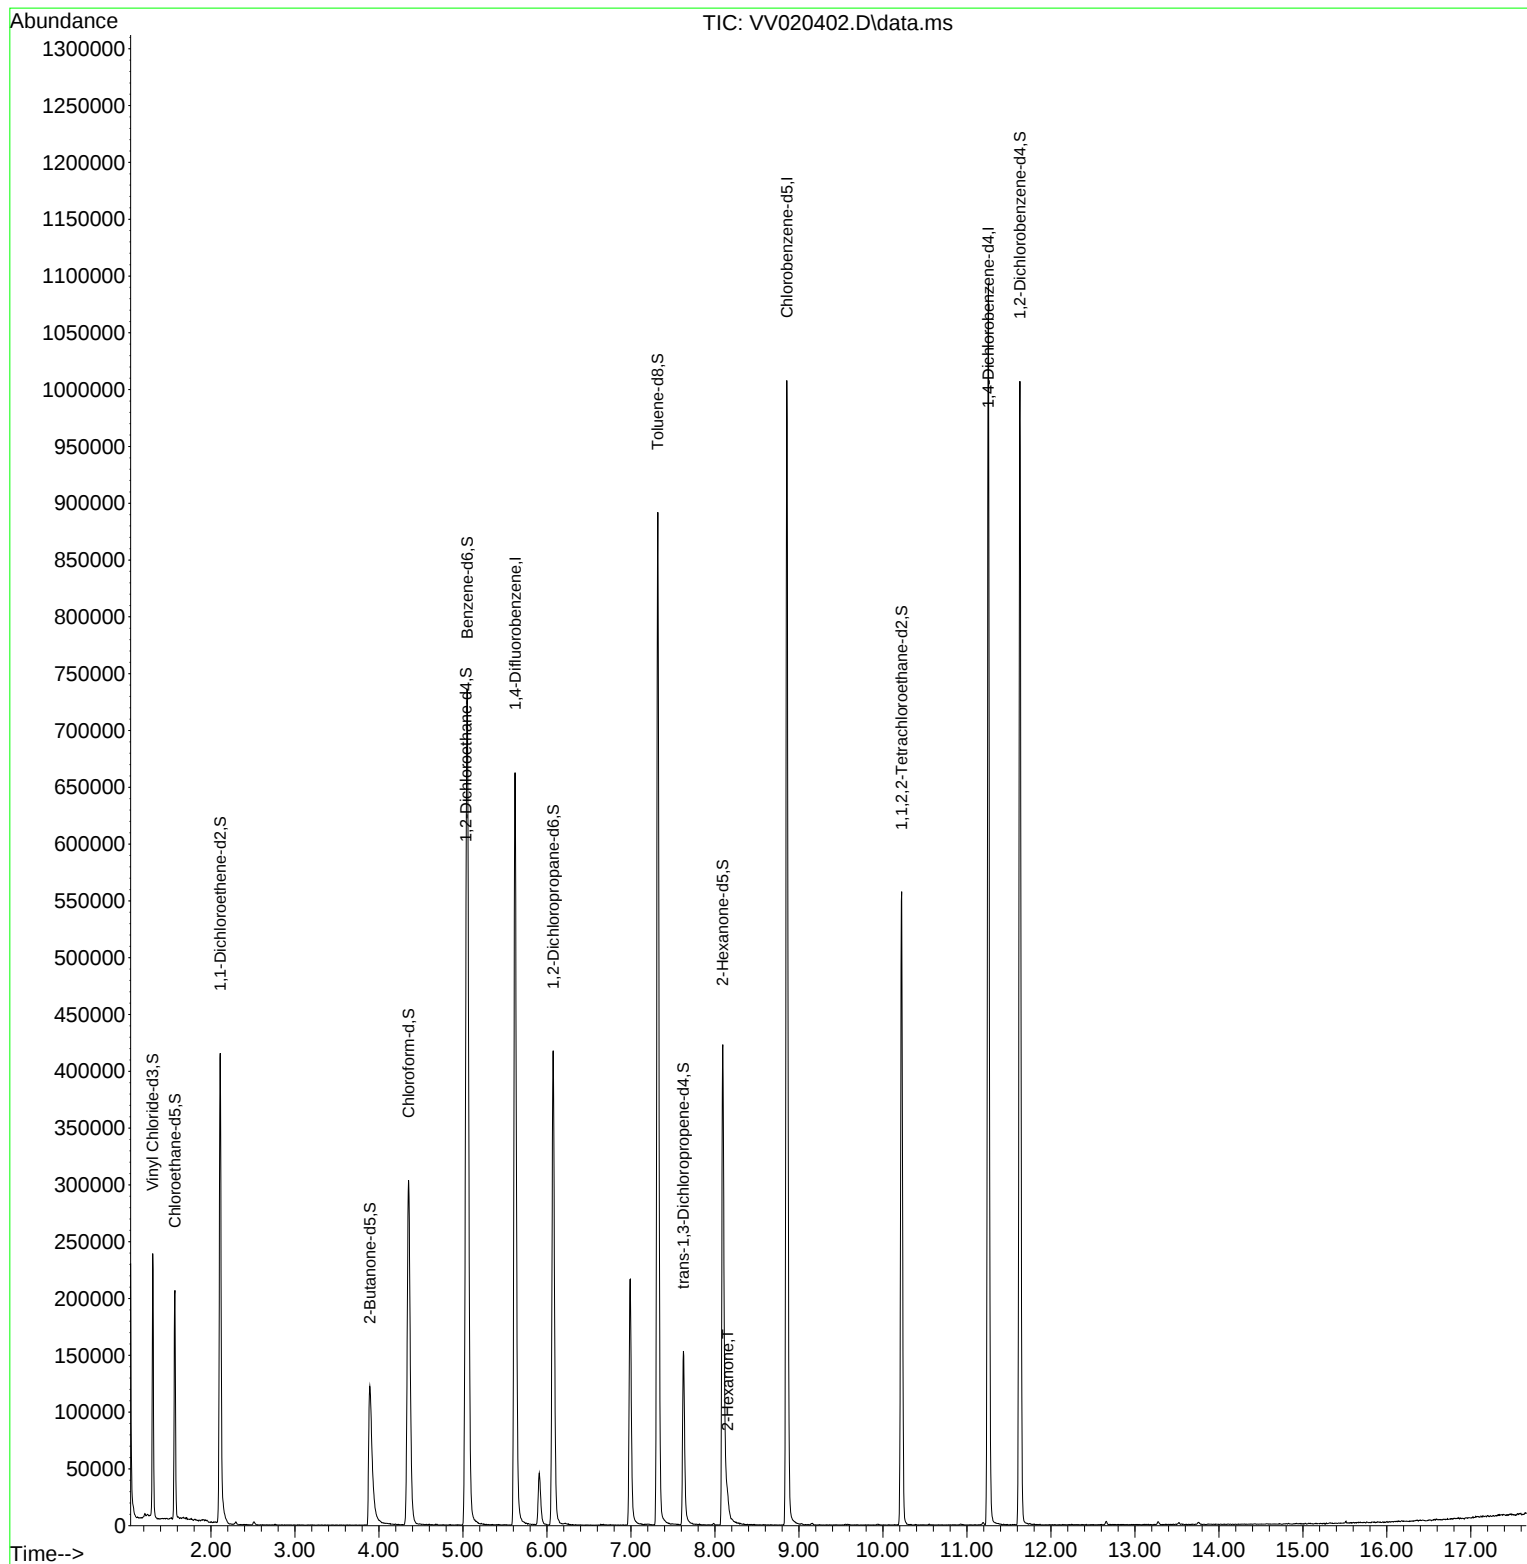

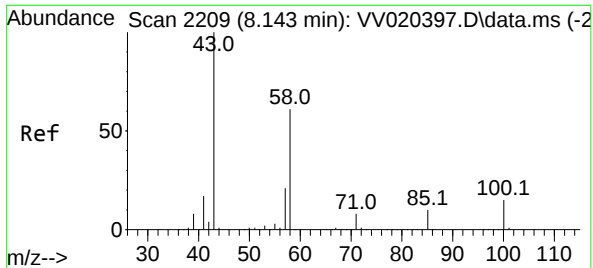

#48
2-Hexanone
Concen: 3.65 ug/L
RT: 8.153 min Scan# 2212
Delta R.T. 0.010 min
Lab File: VV020402.D
Acq: 24 Feb 2021 19:05

Instrument :
MSVOA_V
ClientSampleId :
VBLK167

Tgt Ion: 43	Resp: 12642
Ion Ratio	Lower Upper
43	100
58	48.3 45.3 67.9
57	0.0 15.8 23.6#
100	7.3 10.6 15.8#

