

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022621\
 Data File : VV020401.D
 Acq On : 24 Feb 2021 18:41
 Operator : SY/MD
 Sample : VV0226MBL01
 Misc : 5.0G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK166

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022621WMA.M

Title : VOC Analysis

Signal : TIC: VV020401.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	97	rVB	230980	229692	12.17%	1.502%
2	1.571	157	165	176	rBV	202732	227281	12.04%	1.486%
3	2.108	322	332	363	rVB	418024	642998	34.07%	4.204%
4	2.510	453	457	468	rVB4	2842	4037	0.21%	0.026%
5	2.552	468	470	474	rBV3	289	120	0.01%	0.001%
6	2.767	530	537	545	rBV4	1043	1673	0.09%	0.011%
7	2.863	564	567	568	rBV	273	120	0.01%	0.001%
8	2.921	583	585	589	rVB	386	225	0.01%	0.001%
9	2.950	589	594	595	rBV	263	200	0.01%	0.001%
10	3.034	618	620	622	rBV	248	116	0.01%	0.001%
11	3.220	670	678	681	rBV2	315	433	0.02%	0.003%
12	3.246	681	686	687	rBV2	252	175	0.01%	0.001%
13	3.307	703	705	708	rBV3	227	139	0.01%	0.001%
14	3.330	709	712	715	rBV	196	131	0.01%	0.001%
15	3.368	721	724	726	rBV2	239	123	0.01%	0.001%
16	3.413	736	738	741	rVB	98	45	0.00%	0.000%
17	3.445	746	748	749	rBV	244	76	0.00%	0.000%
18	3.481	756	759	761	rBV2	189	153	0.01%	0.001%
19	3.529	771	774	778	rBV2	267	190	0.01%	0.001%
20	3.552	778	781	782	rBV2	139	77	0.00%	0.001%
21	3.619	800	802	804	rBV	119	77	0.00%	0.001%
22	3.690	819	824	827	rVB2	153	151	0.01%	0.001%
23	3.728	827	836	839	rBV2	368	506	0.03%	0.003%
24	3.761	843	846	852	rVB2	248	273	0.01%	0.002%
25	3.818	862	864	865	rBV	181	64	0.00%	0.000%
26	3.892	876	887	929	rBV2	124423	387135	20.51%	2.531%
27	4.352	1013	1030	1060	rBV	300790	758450	40.19%	4.959%
28	4.658	1120	1125	1128	rBV3	461	426	0.02%	0.003%
29	4.741	1146	1151	1153	rBV2	372	309	0.02%	0.002%
30	4.806	1168	1171	1173	rVB2	234	97	0.01%	0.001%
31	4.822	1173	1176	1179	rBV2	286	231	0.01%	0.002%
32	4.841	1179	1182	1185	rVV4	410	282	0.01%	0.002%
33	4.899	1198	1200	1202	rBV2	221	92	0.00%	0.001%
34	4.931	1206	1210	1213	rVB3	171	126	0.01%	0.001%
35	4.989	1222	1228	1229	rBV2	168	148	0.01%	0.001%
36	5.050	1230	1247	1280	rBV2	738658	1887359	100.00%	12.340%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022621\
 Data File : VV020401.D
 Acq On : 24 Feb 2021 18:41
 Operator : SY/MD
 Sample : VV0226MBL01
 Misc : 5.0G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK166

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022621WMA.M
 Title : VOC Analysis

37	5.355	1339	1342	1344	rBV2	409	260	0.01%	0.002%
38	5.413	1358	1360	1365	rVB2	540	359	0.02%	0.002%
39	5.458	1372	1374	1376	rBV2	347	173	0.01%	0.001%
40	5.503	1384	1388	1394	rVB2	501	474	0.03%	0.003%
41	5.574	1406	1410	1411	rBV	308	219	0.01%	0.001%
42	5.619	1411	1424	1452	rBV	657666	1325926	70.25%	8.669%
43	5.908	1503	1514	1543	rVB	45939	96866	5.13%	0.633%
44	6.072	1551	1565	1599	rBV	415817	845630	44.80%	5.529%
45	6.346	1647	1650	1652	rBV3	237	182	0.01%	0.001%
46	6.371	1656	1658	1662	rBV	211	186	0.01%	0.001%
47	6.436	1675	1678	1680	rVB	229	104	0.01%	0.001%
48	6.445	1680	1681	1683	rBV	226	111	0.01%	0.001%
49	6.477	1689	1691	1695	rBV	174	135	0.01%	0.001%
50	6.500	1696	1698	1702	rVB2	257	156	0.01%	0.001%
51	6.529	1702	1707	1709	rBV2	125	109	0.01%	0.001%
52	6.571	1717	1720	1726	rBV2	305	253	0.01%	0.002%
53	6.603	1727	1730	1734	rVB2	279	196	0.01%	0.001%
54	6.635	1734	1740	1741	rBV2	462	375	0.02%	0.002%
55	6.812	1792	1795	1798	rBV2	195	124	0.01%	0.001%
56	6.857	1807	1809	1814	rVB2	217	117	0.01%	0.001%
57	6.931	1827	1832	1833	rBV	111	83	0.00%	0.001%
58	6.992	1839	1851	1878	rBV	215307	398904	21.14%	2.608%
59	7.320	1939	1953	1975	rBV	899980	1548469	82.04%	10.124%
60	7.625	2038	2048	2074	rBV	152881	269645	14.29%	1.763%
61	7.940	2145	2146	2149	rBV	133	89	0.00%	0.001%
62	7.989	2154	2161	2166	rVV3	1892	2456	0.13%	0.016%
63	8.018	2167	2170	2175	rVB2	416	292	0.02%	0.002%
64	8.092	2183	2193	2235	rBV2	444239	884288	46.85%	5.782%
65	8.532	2328	2330	2332	rBV2	209	125	0.01%	0.001%
66	8.587	2346	2347	2348	rBV	437	115	0.01%	0.001%
67	8.793	2409	2411	2412	rBV	154	71	0.00%	0.000%
68	8.805	2412	2415	2419	rBV	244	166	0.01%	0.001%
69	8.857	2419	2431	2460	rBV	1012863	1642140	87.01%	10.737%
70	9.111	2508	2510	2513	rVB3	442	297	0.02%	0.002%
71	9.146	2513	2521	2522	rBV3	1656	1572	0.08%	0.010%
72	9.255	2552	2555	2562	rBV3	267	274	0.01%	0.002%
73	9.339	2577	2581	2585	rBV2	228	206	0.01%	0.001%
74	9.413	2600	2604	2606	rBV2	161	124	0.01%	0.001%
75	9.426	2606	2608	2611	rVV	293	195	0.01%	0.001%
76	9.458	2615	2618	2622	rBV	267	224	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022621\
 Data File : VV020401.D
 Acq On : 24 Feb 2021 18:41
 Operator : SY/MD
 Sample : VV0226MBL01
 Misc : 5.0G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK166

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022621WMA.M
 Title : VOC Analysis

77	9.551	2643	2647	2652	rBV4	864	844	0.04%	0.006%
78	9.664	2679	2682	2685	rBV	255	178	0.01%	0.001%
79	9.741	2703	2706	2708	rBV	286	194	0.01%	0.001%
80	9.940	2762	2768	2773	rBV3	848	1003	0.05%	0.007%
81	10.053	2802	2803	2804	rBV3	155	56	0.00%	0.000%
82	10.169	2835	2839	2841	rBV2	203	163	0.01%	0.001%
83	10.223	2843	2856	2876	rVV	567822	894060	47.37%	5.846%
84	10.391	2905	2908	2911	rBV2	389	220	0.01%	0.001%
85	10.481	2932	2936	2940	rBV3	393	337	0.02%	0.002%
86	10.921	3069	3073	3075	rBV3	1021	855	0.05%	0.006%
87	10.989	3092	3094	3096	rVB	316	130	0.01%	0.001%
88	11.034	3106	3108	3112	rBV	249	220	0.01%	0.001%
89	11.194	3148	3158	3165	rBV5	1975	3472	0.18%	0.023%
90	11.255	3165	3177	3200	rBV	1086148	1656486	87.77%	10.831%
91	11.632	3282	3294	3314	rBV	1023052	1570778	83.23%	10.270%




Sum of corrected areas: 15294416

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022621\
Data File : VV020401.D
Acq On : 24 Feb 2021 18:41
Operator : SY/MD
Sample : VV0226MBL01
Misc : 5.0G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK166

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

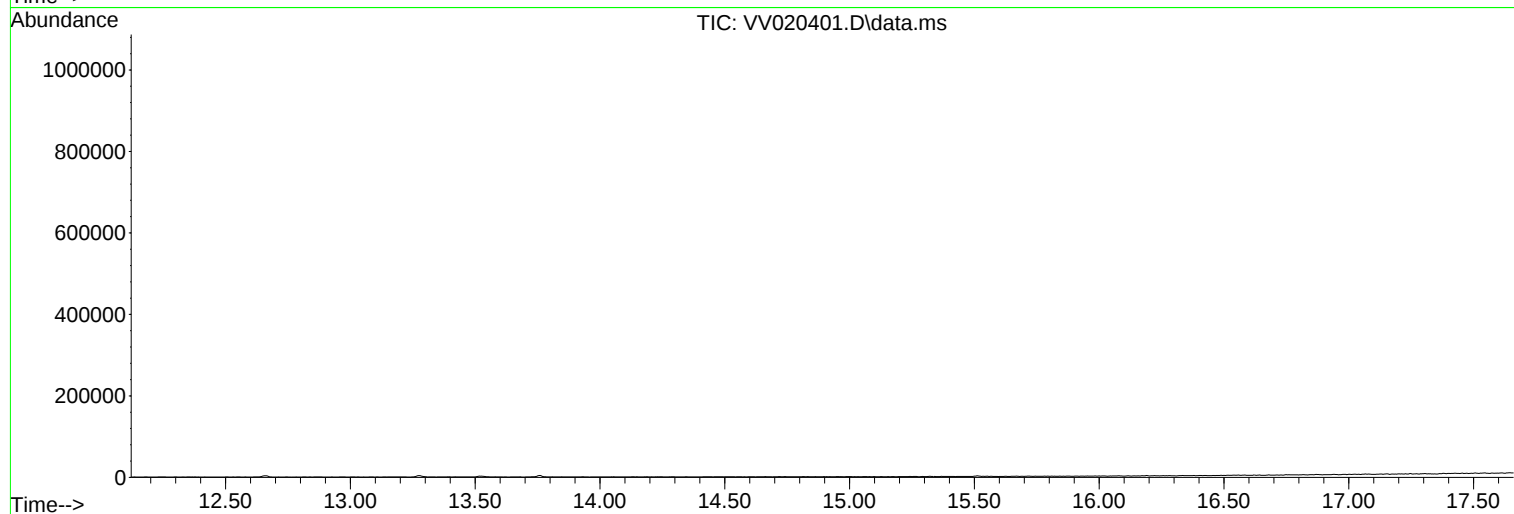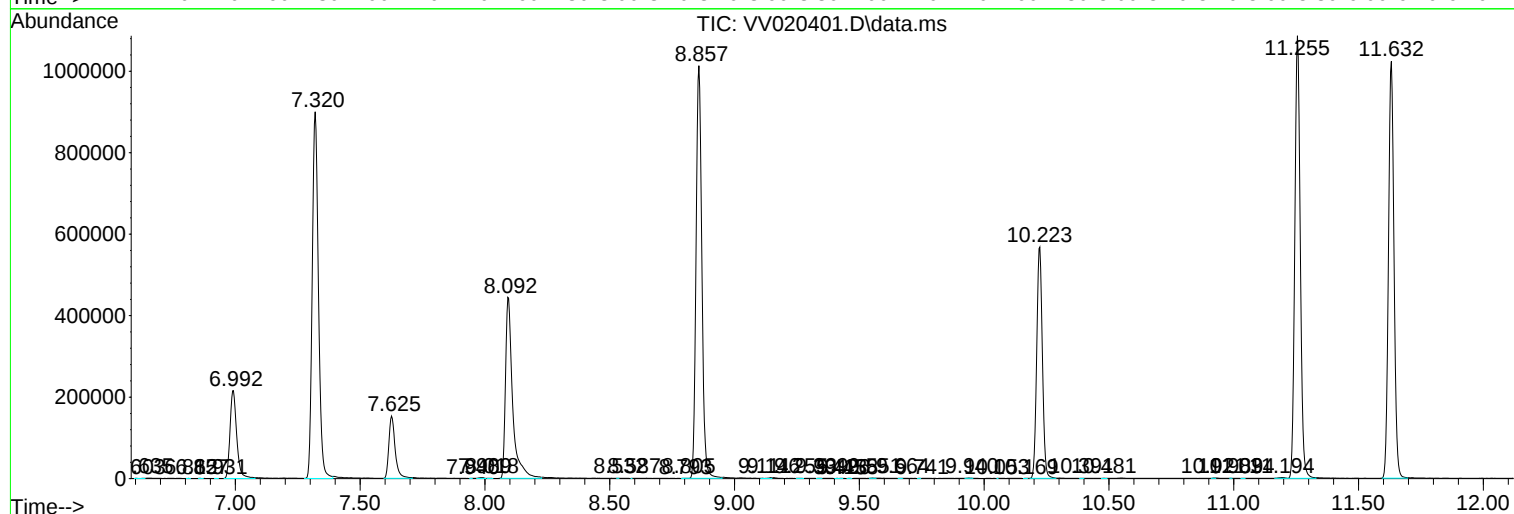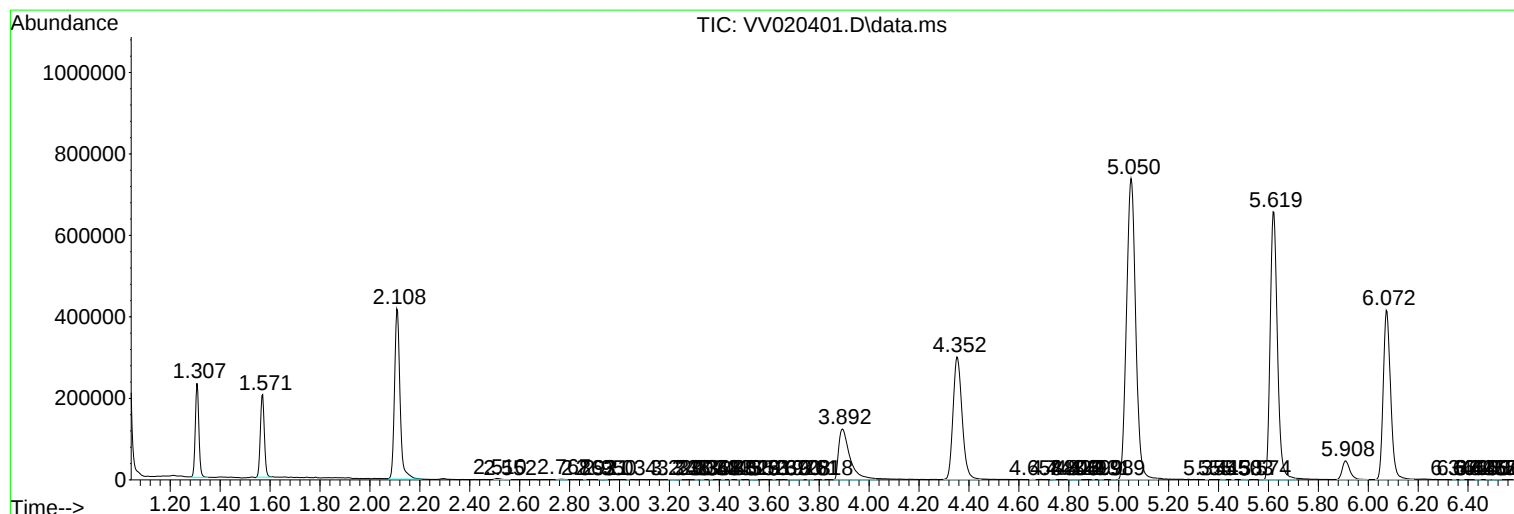

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022621\
Data File : VV020401.D
Acq On : 24 Feb 2021 18:41
Operator : SY/MD
Sample : VV0226MBL01
Misc : 5.0G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK166

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022621\
Data File : VV020401.D
Acq On : 24 Feb 2021 18:41
Operator : SY/MD
Sample : VV0226MBL01
Misc : 5.0G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK166

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
