

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022621\
 Data File : VV020402.D
 Acq On : 24 Feb 2021 19:05
 Operator : SY/MD
 Sample : VV0226WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK167

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022621WMA.M
 Title : VOC Analysis

Signal : TIC: VV020402.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	100	rVB	233688	236352	12.55%	1.551%
2	1.571	157	165	175	rBV	200811	227576	12.09%	1.493%
3	2.111	322	333	364	rVB	414179	639955	33.99%	4.199%
4	2.297	382	391	401	rVB3	2743	4608	0.24%	0.030%
5	2.426	428	431	434	rVB3	332	221	0.01%	0.001%
6	2.513	449	458	470	rVB3	2603	4220	0.22%	0.028%
7	2.590	478	482	486	rBV2	354	360	0.02%	0.002%
8	2.664	502	505	510	rVB2	369	330	0.02%	0.002%
9	2.693	510	514	516	rBV3	304	228	0.01%	0.001%
10	2.760	534	535	542	rVB3	599	502	0.03%	0.003%
11	2.998	602	609	612	rBV2	301	376	0.02%	0.002%
12	3.140	646	653	655	rBV	157	214	0.01%	0.001%
13	3.317	705	708	715	rVB3	335	365	0.02%	0.002%
14	3.484	757	760	763	rBV2	314	249	0.01%	0.002%
15	3.551	777	781	787	rVV3	298	255	0.01%	0.002%
16	3.651	808	812	818	rVB2	217	215	0.01%	0.001%
17	3.892	876	887	921	rBV2	122073	367308	19.51%	2.410%
18	4.195	978	981	985	rVB2	459	268	0.01%	0.002%
19	4.352	1013	1030	1061	rBV2	303138	758289	40.27%	4.975%
20	4.677	1124	1131	1134	rBV3	662	710	0.04%	0.005%
21	4.844	1179	1183	1188	rVB3	553	523	0.03%	0.003%
22	4.873	1188	1192	1195	rBV3	258	230	0.01%	0.002%
23	4.953	1213	1217	1220	rVB3	250	207	0.01%	0.001%
24	5.050	1227	1247	1275	rBV2	736103	1882842	100.00%	12.354%
25	5.217	1297	1299	1303	rVB5	728	415	0.02%	0.003%
26	5.352	1338	1341	1344	rVB3	373	221	0.01%	0.001%
27	5.490	1379	1384	1385	rBV	362	274	0.01%	0.002%
28	5.622	1412	1425	1463	rVV	662069	1322896	70.26%	8.680%
29	5.776	1471	1473	1479	rVB3	642	425	0.02%	0.003%
30	5.908	1501	1514	1535	rBV2	45373	96270	5.11%	0.632%
31	6.075	1552	1566	1599	rBV	417322	841035	44.67%	5.518%
32	6.342	1645	1649	1654	rBV2	494	353	0.02%	0.002%
33	6.638	1738	1741	1744	rBV2	660	434	0.02%	0.003%
34	6.654	1744	1746	1750	rVV2	555	468	0.02%	0.003%
35	6.674	1750	1752	1756	rVV3	606	479	0.03%	0.003%
36	6.992	1838	1851	1879	rBV2	216429	398014	21.14%	2.611%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022621\
 Data File : VV020402.D
 Acq On : 24 Feb 2021 19:05
 Operator : SY/MD
 Sample : VV0226WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK167

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022621WMA.M
 Title : VOC Analysis

37	7.156	1899	1902	1905	rVB2	372	246	0.01%	0.002%
38	7.178	1905	1909	1912	rBV2	500	521	0.03%	0.003%
39	7.320	1941	1953	1990	rBV	891312	1540631	81.82%	10.109%
40	7.625	2038	2048	2078	rBV	152829	271247	14.41%	1.780%
41	7.812	2104	2106	2114	rVB6	581	583	0.03%	0.004%
42	7.921	2132	2140	2142	rBV4	399	439	0.02%	0.003%
43	7.982	2154	2159	2167	rVB3	1342	1787	0.09%	0.012%
44	8.095	2183	2194	2236	rBV2	422783	852836	45.30%	5.596%
45	8.336	2267	2269	2273	rVB3	396	241	0.01%	0.002%
46	8.461	2304	2308	2310	rBV3	403	260	0.01%	0.002%
47	8.577	2340	2344	2347	rBV2	326	217	0.01%	0.001%
48	8.632	2359	2361	2367	rVB3	332	272	0.01%	0.002%
49	8.667	2367	2372	2375	rBV3	451	411	0.02%	0.003%
50	8.857	2419	2431	2453	rBV	1007317	1631833	86.67%	10.707%
51	9.079	2496	2500	2502	rBV3	362	269	0.01%	0.002%
52	9.107	2506	2509	2513	rVV2	379	312	0.02%	0.002%
53	9.159	2517	2525	2536	rVV6	1437	2546	0.14%	0.017%
54	9.249	2548	2553	2557	rBV2	426	323	0.02%	0.002%
55	9.333	2577	2579	2584	rVB	432	306	0.02%	0.002%
56	9.368	2584	2590	2592	rBV	382	407	0.02%	0.003%
57	9.429	2604	2609	2613	rBV2	218	249	0.01%	0.002%
58	9.551	2642	2647	2648	rBV	592	403	0.02%	0.003%
59	9.580	2653	2656	2658	rBV	438	309	0.02%	0.002%
60	9.744	2699	2707	2713	rBV2	286	456	0.02%	0.003%
61	9.821	2728	2731	2737	rVB2	238	249	0.01%	0.002%
62	9.931	2762	2765	2766	rBV	537	347	0.02%	0.002%
63	10.008	2785	2789	2791	rBV2	311	253	0.01%	0.002%
64	10.136	2826	2829	2834	rBV2	306	249	0.01%	0.002%
65	10.223	2843	2856	2883	rVV	557332	879916	46.73%	5.773%
66	10.384	2903	2906	2908	rBV3	457	296	0.02%	0.002%
67	10.551	2952	2958	2963	rBV4	752	849	0.05%	0.006%
68	10.837	3040	3047	3050	rBV2	213	281	0.01%	0.002%
69	10.924	3069	3074	3079	rBV3	724	940	0.05%	0.006%
70	10.960	3083	3085	3090	rVB	417	262	0.01%	0.002%
71	11.095	3125	3127	3133	rVV3	306	277	0.01%	0.002%
72	11.175	3148	3152	3153	rBV2	444	287	0.02%	0.002%
73	11.191	3153	3157	3165	rVB4	1946	2473	0.13%	0.016%
74	11.255	3165	3177	3201	rBV	1092602	1655160	87.91%	10.860%
75	11.480	3245	3247	3252	rVB2	503	331	0.02%	0.002%
76	11.632	3281	3294	3315	rBV	1006660	1583869	84.12%	10.392%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022621\
 Data File : VV020402.D
 Acq On : 24 Feb 2021 19:05
 Operator : SY/MD
 Sample : VV0226WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK167

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022621WMA.M
 Title : VOC Analysis

77	12.098	3436	3439	3442	rVB3	325	226	0.01%	0.001%
78	12.140	3449	3452	3456	rBV2	337	298	0.02%	0.002%
79	12.210	3471	3474	3478	rBV2	274	260	0.01%	0.002%
80	12.448	3541	3548	3550	rBV	246	340	0.02%	0.002%
81	12.657	3606	3613	3625	rVB6	2901	4180	0.22%	0.027%
82	12.705	3625	3628	3630	rBV	401	265	0.01%	0.002%
83	13.046	3731	3734	3738	rBV3	333	290	0.02%	0.002%
84	13.188	3773	3778	3786	rBV2	337	454	0.02%	0.003%
85	13.230	3787	3791	3793	rBV3	412	332	0.02%	0.002%
86	13.278	3800	3806	3815	rVB7	2575	3563	0.19%	0.023%
87	13.490	3867	3872	3874	rBV3	349	315	0.02%	0.002%
88	13.503	3874	3876	3878	rBV	614	369	0.02%	0.002%
89	13.525	3880	3883	3889	rVB2	1676	1618	0.09%	0.011%
90	13.638	3915	3918	3919	rBV	406	236	0.01%	0.002%
91	13.718	3940	3943	3948	rBV2	357	444	0.02%	0.003%
92	13.760	3948	3956	3964	rVB5	1868	3073	0.16%	0.020%
93	13.869	3988	3990	3993	rVB	405	220	0.01%	0.001%
94	13.905	3999	4001	4006	rVB2	375	258	0.01%	0.002%
95	14.111	4061	4065	4070	rBV3	550	502	0.03%	0.003%
96	14.770	4267	4270	4273	rBV2	448	379	0.02%	0.002%
97	14.889	4303	4307	4308	rBV2	419	300	0.02%	0.002%
98	15.030	4348	4351	4355	rVB3	644	510	0.03%	0.003%
99	15.281	4427	4429	4434	rBV3	675	342	0.02%	0.002%
100	15.512	4497	4501	4505	rVB5	1679	1282	0.07%	0.008%


Sum of corrected areas: 15240886

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022621\
Data File : VV020402.D
Acq On : 24 Feb 2021 19:05
Operator : SY/MD
Sample : VV0226WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK167

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

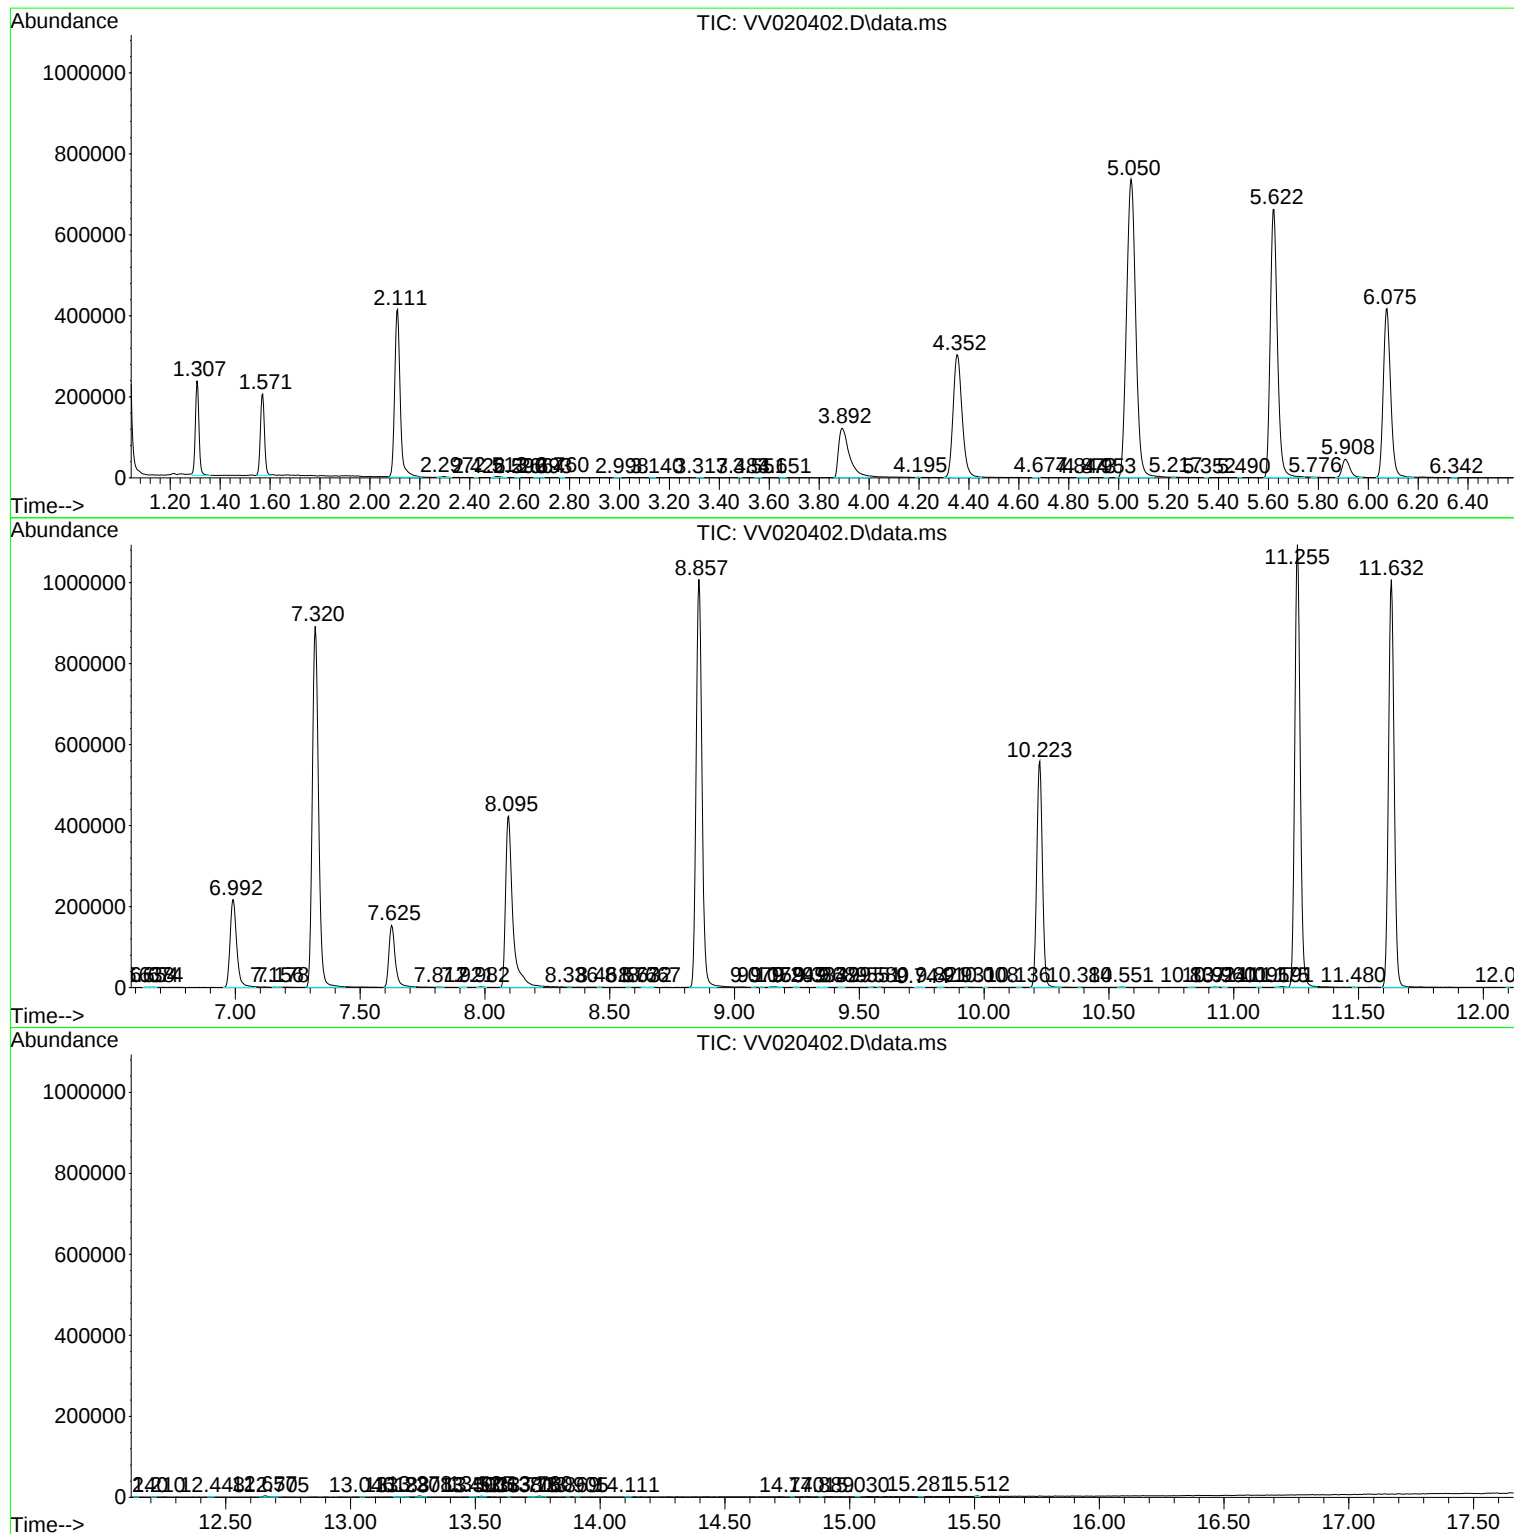

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022621\
Data File : VV020402.D
Acq On : 24 Feb 2021 19:05
Operator : SY/MD
Sample : VV0226WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK167

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022621\
Data File : VV020402.D
Acq On : 24 Feb 2021 19:05
Operator : SY/MD
Sample : VV0226WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK167

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
