
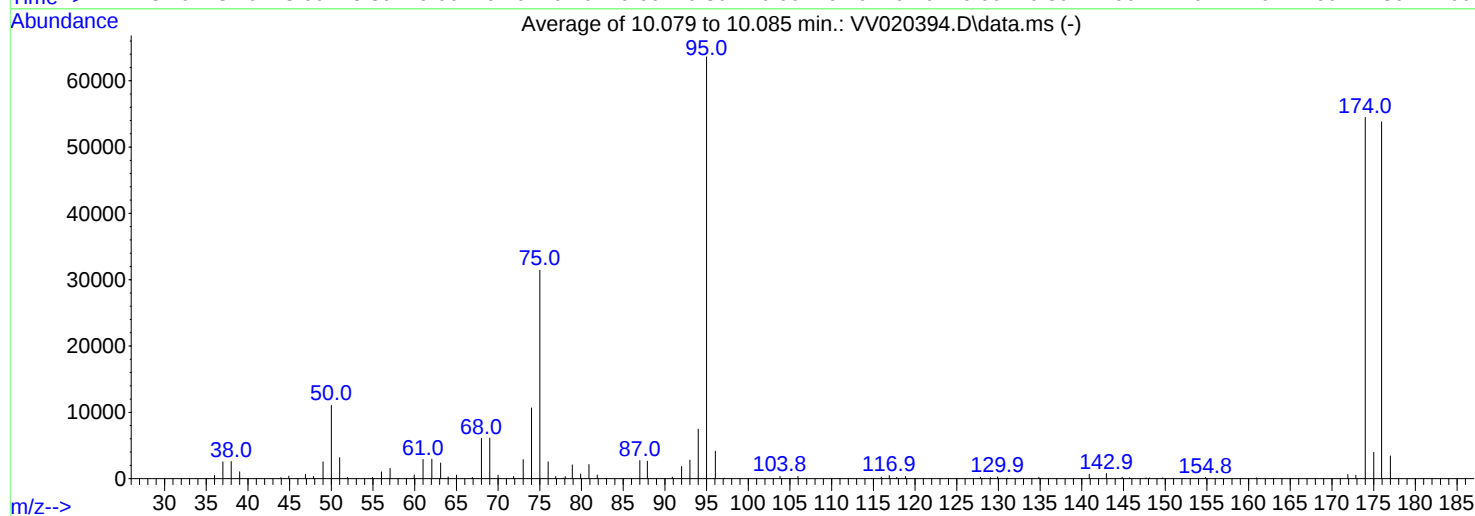


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022621\
 Data File : VV020394.D
 Acq On : 24 Feb 2021 14:10
 Operator : SY/MD
 Sample : BFB86
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB86

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022621WMA.M
 Title : VOC Analysis
 Last Update : Wed Feb 24 17:44:20 2021

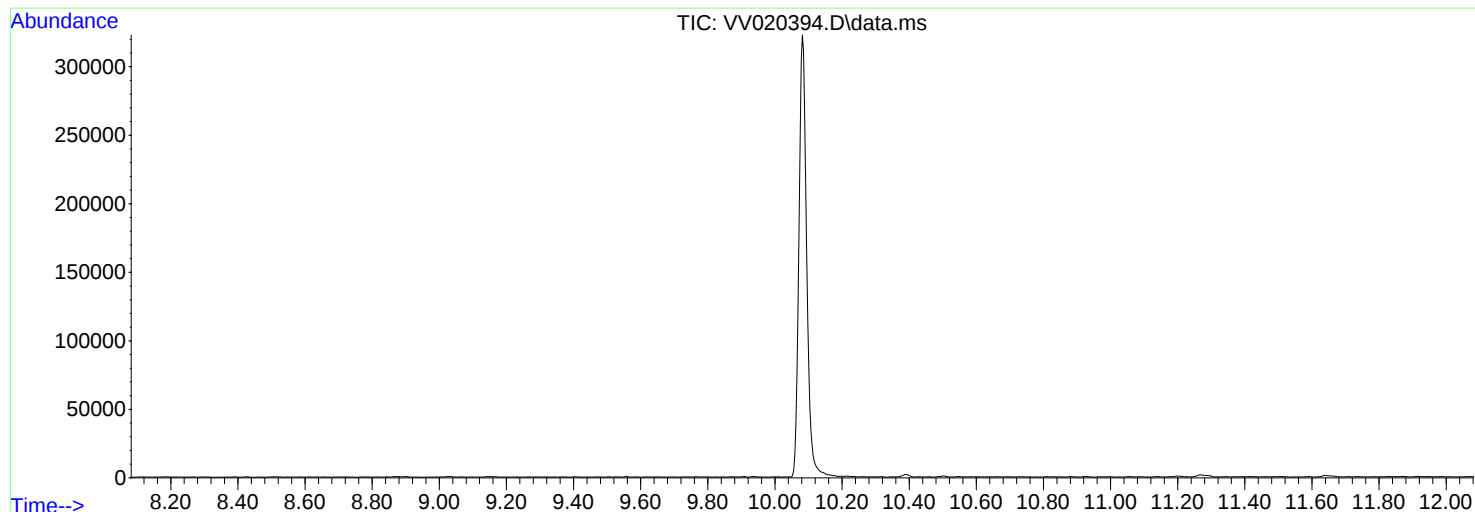

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	11060	PASS
75	95	30	80	49.4	31427	PASS
95	95	100	100	100.0	63605	PASS
96	95	5	9	6.5	4141	PASS
173	174	0.00	2	0.9	500	PASS
174	95	50	120	85.6	54475	PASS
175	174	5	9	7.3	3966	PASS
176	174	95	101	98.8	53797	PASS
177	176	5	9	6.4	3434	PASS

m/z	Abundance
36.00	543.0
37.00	2781.0
38.00	2502.0
39.00	976.0
40.10	234.0
44.00	704.0
44.90	381.0
46.90	724.0
47.80	305.0
49.00	2488.0
50.00	11178.0
51.00	3176.0
51.90	149.0
54.90	176.0
56.00	1051.0
57.00	1474.0
60.00	508.0
61.00	2965.0
62.00	2843.0
63.10	2280.0
64.00	304.0
65.00	480.0
66.90	203.0
68.00	6039.0
69.00	5853.0
70.00	571.0
71.80	348.0
73.00	2832.0
74.00	10408.0
75.00	30920.0
76.00	2644.0
76.90	248.0
77.80	256.0
78.00	259.0
78.90	1973.0
79.90	730.0
80.90	1972.0
81.90	525.0
87.00	2695.0
87.90	2443.0
90.90	234.0
92.00	1863.0
93.00	2849.0
94.00	7321.0
95.00	62536.0
96.00	4097.0
97.10	164.0
103.80	342.0
104.50	100.0
105.90	310.0
110.90	106.0
115.90	251.0
116.90	443.0
117.70	222.0
118.90	343.0
127.90	266.0
129.00	114.0
129.90	258.0
131.10	103.0
134.90	132.0
140.90	677.0
142.90	729.0
144.80	188.0
145.70	151.0
147.70	117.0
148.10	117.0
149.70	131.0
154.90	176.0
156.80	116.0
161.00	129.0
171.90	598.0
172.80	454.0
174.00	50912.0
175.00	3621.0
176.00	51624.0
177.00	3516.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
36.00	486.0
37.00	2623.0
38.00	2689.0
39.00	1095.0
40.10	233.0
44.10	672.0
44.90	381.0
46.90	680.0
47.90	338.0
49.00	2643.0
50.00	11482.0
51.00	3262.0
52.00	181.0
55.00	198.0
56.00	1071.0
57.00	1593.0
59.90	575.0
61.00	2983.0
62.00	3017.0
63.10	2489.0
64.00	269.0
65.00	567.0
66.90	196.0
68.00	6283.0
69.00	6282.0
70.00	558.0
71.80	343.0
73.00	2932.0
74.00	11035.0
75.00	32544.0
76.00	2574.0
76.90	310.0
78.10	313.0
78.90	2169.0
79.90	712.0
80.90	2182.0
81.90	581.0
87.00	2840.0
87.90	2739.0
90.90	264.0
92.00	1863.0
93.00	2906.0
94.00	7656.0
95.00	65736.0
96.10	4246.0
97.10	135.0
103.80	391.0
106.00	325.0
116.00	243.0
116.90	454.0
117.80	190.0
118.90	357.0
127.90	257.0
129.00	155.0
129.90	263.0
131.10	107.0
134.80	208.0
140.90	679.0
143.00	781.0
144.90	210.0
145.70	159.0
147.70	122.0
148.10	105.0
149.70	145.0
154.90	198.0
161.00	124.0
171.90	651.0
172.80	517.0
174.00	56240.0
175.00	4157.0
175.90	55552.0
177.00	3634.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
36.00	396.0
37.00	2188.0
38.00	2543.0
39.00	1074.0
40.10	265.0
44.10	639.0
44.90	369.0
46.90	551.0
47.90	355.0
49.00	2505.0
50.00	10521.0
51.00	3069.0
52.00	204.0
55.00	188.0
56.00	915.0
57.10	1543.0
59.90	584.0
61.00	2704.0
62.10	2960.0
63.10	2369.0
64.00	235.0
65.00	552.0
66.90	167.0
68.00	5918.0
69.00	6223.0
70.00	497.0
71.90	305.0
73.00	2861.0
74.00	10593.0
75.00	30816.0
76.00	2383.0
76.90	363.0
78.10	283.0
78.90	2084.0
79.90	646.0
80.90	2211.0
81.90	586.0
82.90	103.0
87.00	2666.0
87.90	2722.0
90.90	259.0
92.00	1808.0
93.00	2622.0
94.00	7375.0
95.00	62544.0
96.00	4080.0
103.80	364.0
105.00	103.0
106.00	352.0
114.80	102.0
116.00	211.0
116.90	447.0
117.90	183.0
118.80	353.0
127.80	212.0
129.10	183.0
129.90	277.0
134.80	258.0
140.90	648.0
142.90	791.0
144.90	257.0
145.70	126.0
147.70	118.0
148.10	113.0
149.70	111.0
154.80	210.0
160.90	139.0
171.90	625.0
172.90	530.0
174.00	56272.0
175.00	4121.0
175.90	54216.0
177.00	3153.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
39.90	224.0
43.90	489.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86