

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022624\
 Data File : VW034429.D
 Acq On : 26 Feb 2024 23:55
 Operator : SY/MD
 Sample : P1535-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF8

Quant Time: Feb 27 05:11:23 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Feb 27 05:05:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	55118	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	54274	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	25630	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	16286	5.090	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	101.800%	
7) Chloroethane-d5	1.532	69	14468	5.120	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	102.400%	
11) 1,1-Dichloroethene-d2	2.060	65	7947	5.336	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	106.800%	
20) 2-Butanone-d5	3.789	46	92043	110.028	ug/L	-0.03
Spiked Amount	50.000	Range 40 - 130	Recovery	=	220.060%#	
24) Chloroform-d	4.256	84	32536	5.065	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.200%	
26) 1,2-Dichloroethane-d4	4.950	65	22934	7.015	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	140.400%#	
32) Benzene-d6	4.966	84	61016	4.997	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.000%	
36) 1,2-Dichloropropane-d6	5.992	67	19038	5.222	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	104.400%	
41) Toluene-d8	7.249	98	50909	4.650	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	93.000%	
43) trans-1,3-Dichloroprop...	7.567	79	7752	5.708	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	114.200%	
46) 2-Hexanone-d5	8.024	63	75244	97.982	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	195.960%#	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	23200	8.040	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	160.800%#	
66) 1,2-Dichlorobenzene-d4	11.564	152	22823	5.861	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	117.200%	
Target Compounds						Qvalue
22) cis-1,2-Dichloroethene	3.831	96	2622	0.679	ug/L	94
25) Chloroform	4.285	83	5460	0.778	ug/L	98
31) Carbon tetrachloride	4.741	117	9083	1.541	ug/L	100
34) Trichloroethene	5.838	95	10262	2.616	ug/L	94
47) Tetrachloroethene	7.908	164	18192	5.912	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022624\
Data File : VV034429.D
Acq On : 26 Feb 2024 23:55
Operator : SY/MD
Sample : P1535-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF8

Quant Time: Feb 27 05:11:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Feb 27 05:05:59 2024
Response via : Initial Calibration




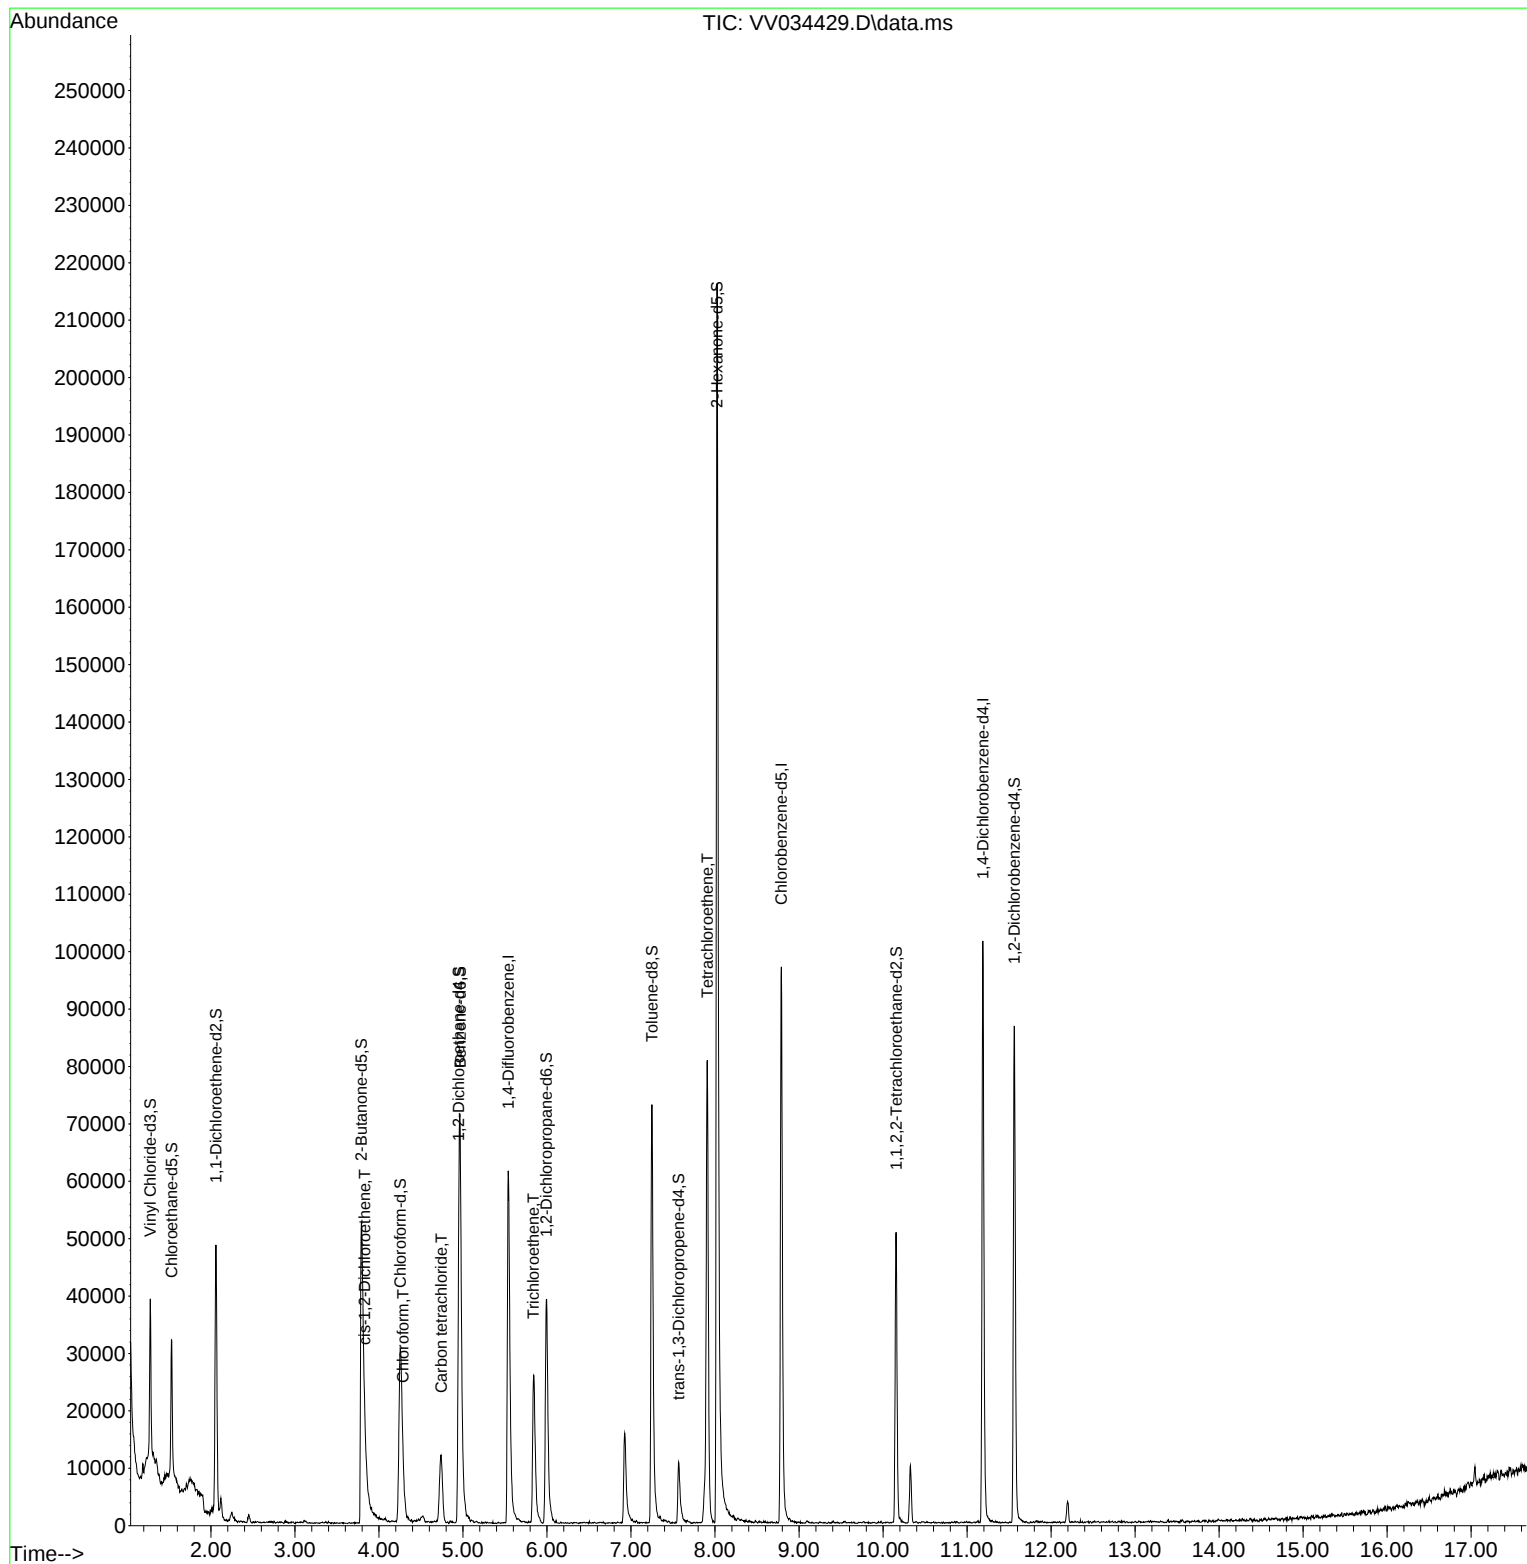


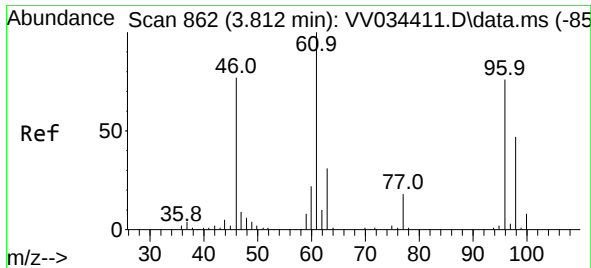

#22
 cis-1,2-Dichloroethene
 Concen: 0.679 ug/L
 RT: 3.831 min Scan# 80
 Delta R.T. 0.019 min
 Lab File: VV034429.D
 Acq: 26 Feb 2024 23:55




Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF8


Tgt Ion: 96 Resp: 2622
 Ion Ratio Lower Upper
 96 100
 61 126.5 89.7 166.5
 98 72.8 42.0 78.0

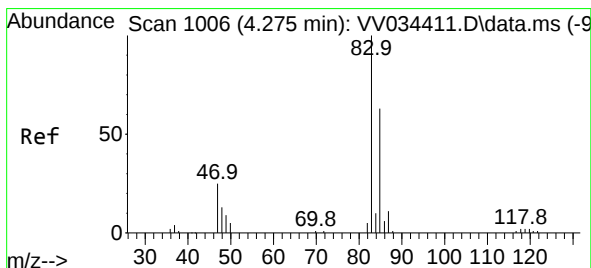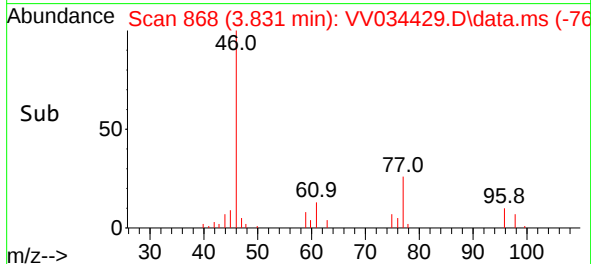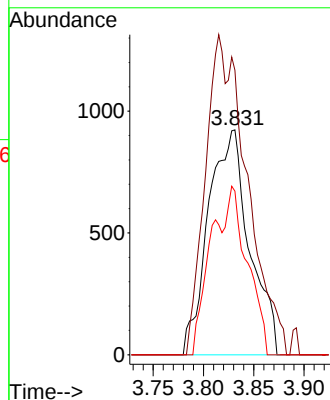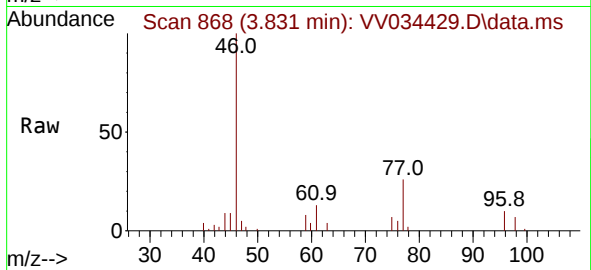

#25
 Chloroform
 Concen: 0.778 ug/L
 RT: 4.285 min Scan# 1009
 Delta R.T. 0.010 min
 Lab File: VV034429.D
 Acq: 26 Feb 2024 23:55

Tgt Ion: 83 Resp: 5460
 Ion Ratio Lower Upper
 83 100
 85 65.7 47.0 87.4


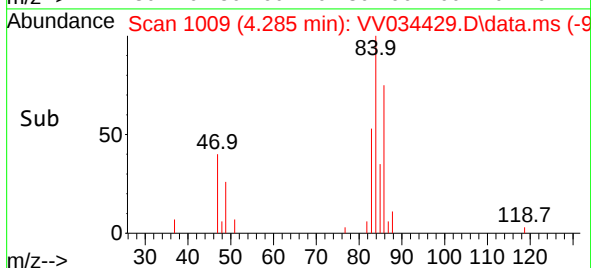
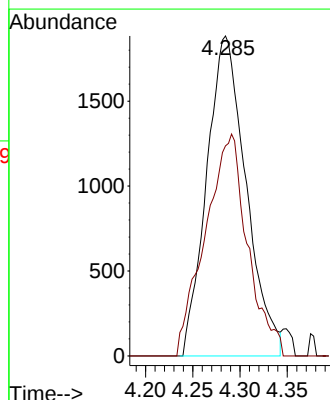
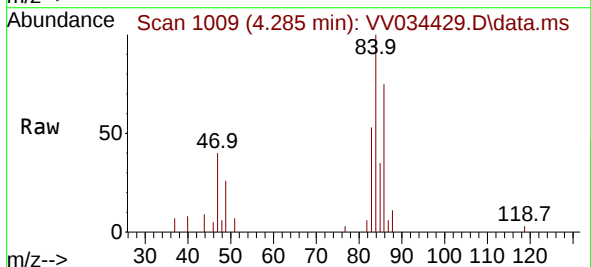


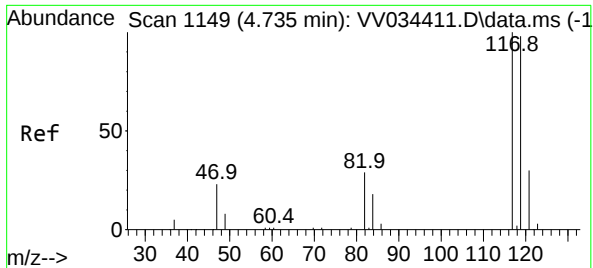

#31
Carbon tetrachloride
Concen: 1.541 ug/L
RT: 4.741 min Scan# 1149
Delta R.T. 0.007 min
Lab File: VV034429.D
Acq: 26 Feb 2024 23:55




Instrument :
MSVOA_V
ClientSampleId :
C0AF8


Tgt Ion:117 Resp: 9083
Ion Ratio Lower Upper
117 100
119 96.0 77.0 115.6

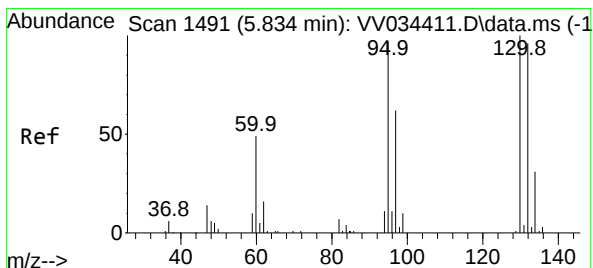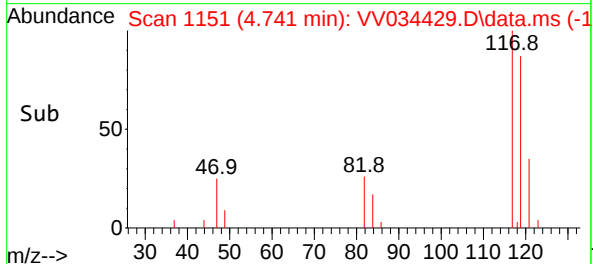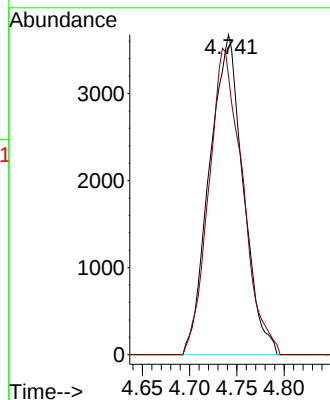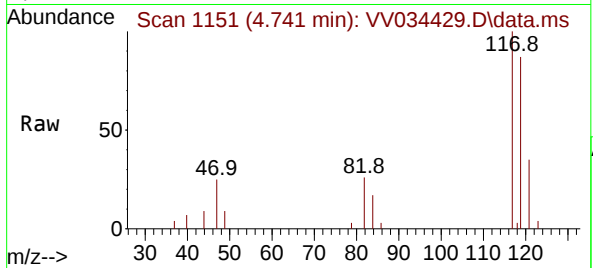

#34
Trichloroethene
Concen: 2.616 ug/L
RT: 5.838 min Scan# 1492
Delta R.T. 0.003 min
Lab File: VV034429.D
Acq: 26 Feb 2024 23:55


Tgt Ion: 95 Resp: 10262
Ion Ratio Lower Upper
95 100
97 54.3 43.3 80.5
132 89.7 67.8 126.0
130 102.8 70.3 130.5

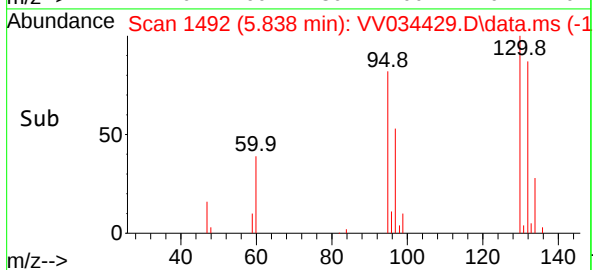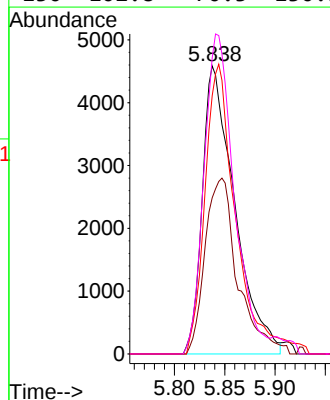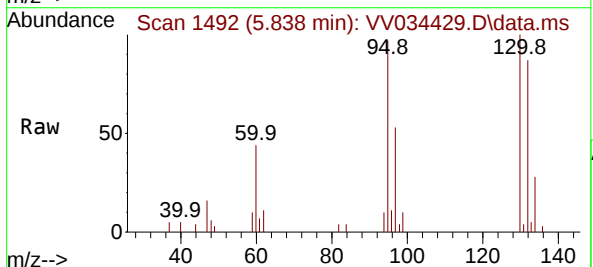

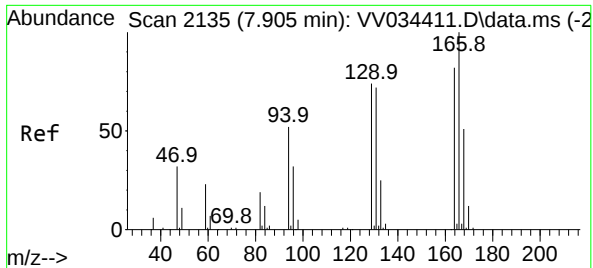

#47
Tetrachloroethene
Concen: 5.912 ug/L
RT: 7.908 min Scan# 21
Delta R.T. 0.003 min
Lab File: VV034429.D
Acq: 26 Feb 2024 23:55

Instrument :
MSVOA_V
ClientSampleId :
C0AF8

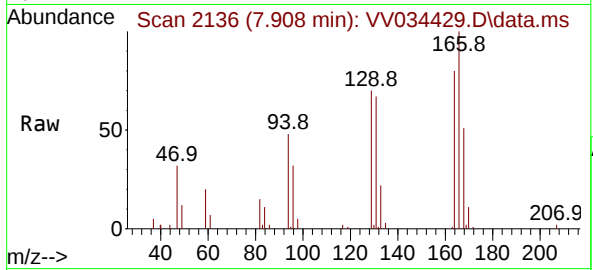

Tgt Ion:	164	Resp:	18192
Ion	Ratio	Lower	Upper
164	100		
129	87.9	64.2	119.2
131	83.4	65.9	122.3
166	125.3	89.9	166.9

