

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022624\
 Data File : VV034413.D
 Acq On : 26 Feb 2024 17:30
 Operator : SY/MD
 Sample : P1503-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCNC6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV034413.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	68646	88099	15.76%	1.926%
2	1.532	147	153	166	rVB	62447	78082	13.96%	1.707%
3	2.060	307	317	332	rVB	115185	178047	31.84%	3.892%
4	2.706	504	518	541	rBV2	93196	196011	35.05%	4.285%
5	3.677	804	820	831	rVB4	2717	6330	1.13%	0.138%
6	3.812	850	862	904	rBV	66302	236181	42.24%	5.163%
7	4.252	983	999	1021	rBV2	77272	198002	35.41%	4.328%
8	4.960	1205	1219	1252	rBV2	170076	440579	78.79%	9.631%
9	5.207	1284	1296	1308	rBV4	6126	13747	2.46%	0.301%
10	5.535	1387	1398	1436	rBV	161155	340418	60.88%	7.442%
11	5.992	1528	1540	1564	rBV2	100598	213074	38.11%	4.658%
12	6.918	1819	1828	1852	rBV2	43843	87189	15.59%	1.906%
13	7.246	1919	1930	1955	rBV	194511	354720	63.44%	7.754%
14	7.561	2019	2028	2048	rBV	26029	48585	8.69%	1.062%
15	7.876	2114	2126	2142	rVB2	24412	44001	7.87%	0.962%
16	8.024	2163	2172	2206	rBV	307891	559158	100.00%	12.223%
17	8.786	2399	2409	2435	rBV	251111	417225	74.62%	9.121%
18	9.082	2489	2501	2512	rBV	10597	18032	3.22%	0.394%
19	10.153	2823	2834	2852	rBV	83975	134998	24.14%	2.951%
20	10.326	2877	2888	2901	rBV2	38654	63145	11.29%	1.380%
21	11.188	3144	3156	3178	rBV	271238	425773	76.15%	9.307%
22	11.468	3234	3243	3252	rBV	11201	16793	3.00%	0.367%
23	11.561	3261	3272	3295	rBV	220438	356588	63.77%	7.795%
24	12.197	3459	3470	3481	rVB	13161	21515	3.85%	0.470%
25	15.332	4438	4445	4452	rBV7	5019	6567	1.17%	0.144%
26	16.249	4722	4730	4739	rBV3	13997	19514	3.49%	0.427%
27	17.043	4970	4977	4988	rVB	7678	12156	2.17%	0.266%




Sum of corrected areas: 4574529

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022624\
Data File : VV034413.D
Acq On : 26 Feb 2024 17:30
Operator : SY/MD
Sample : P1503-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

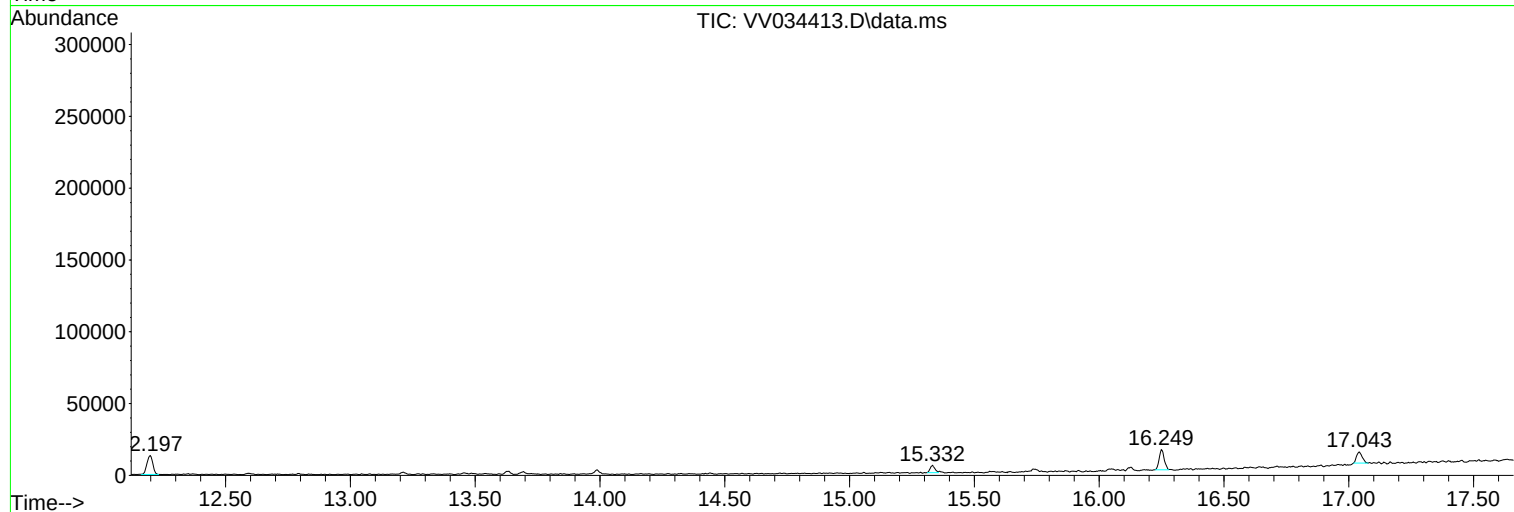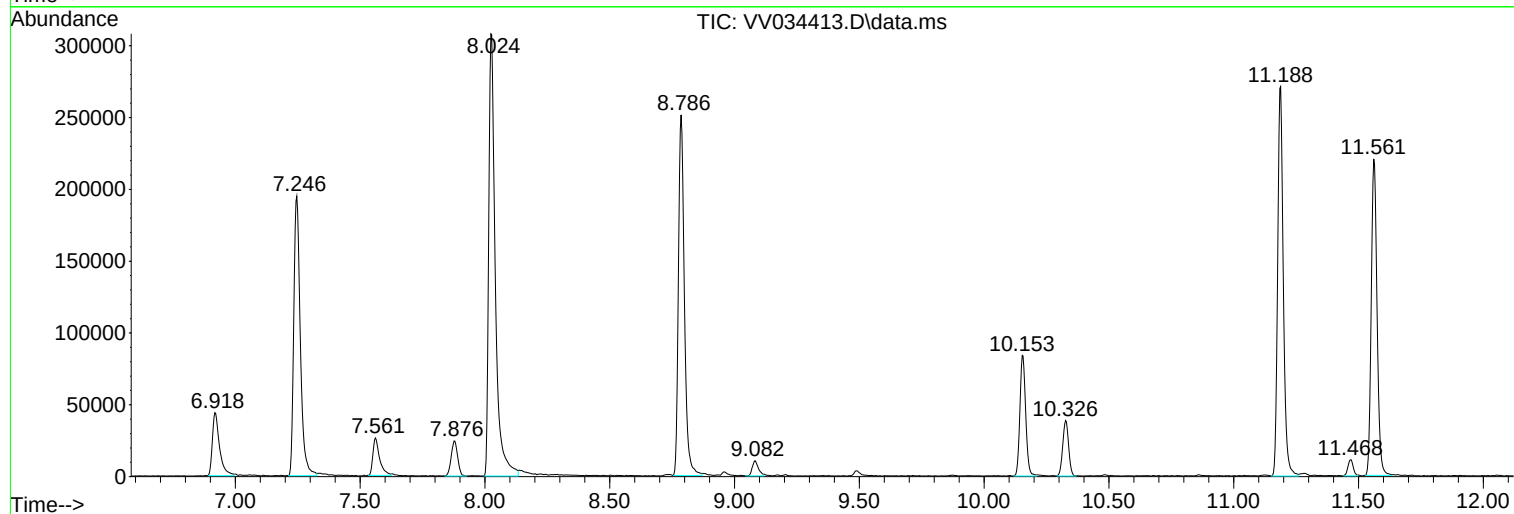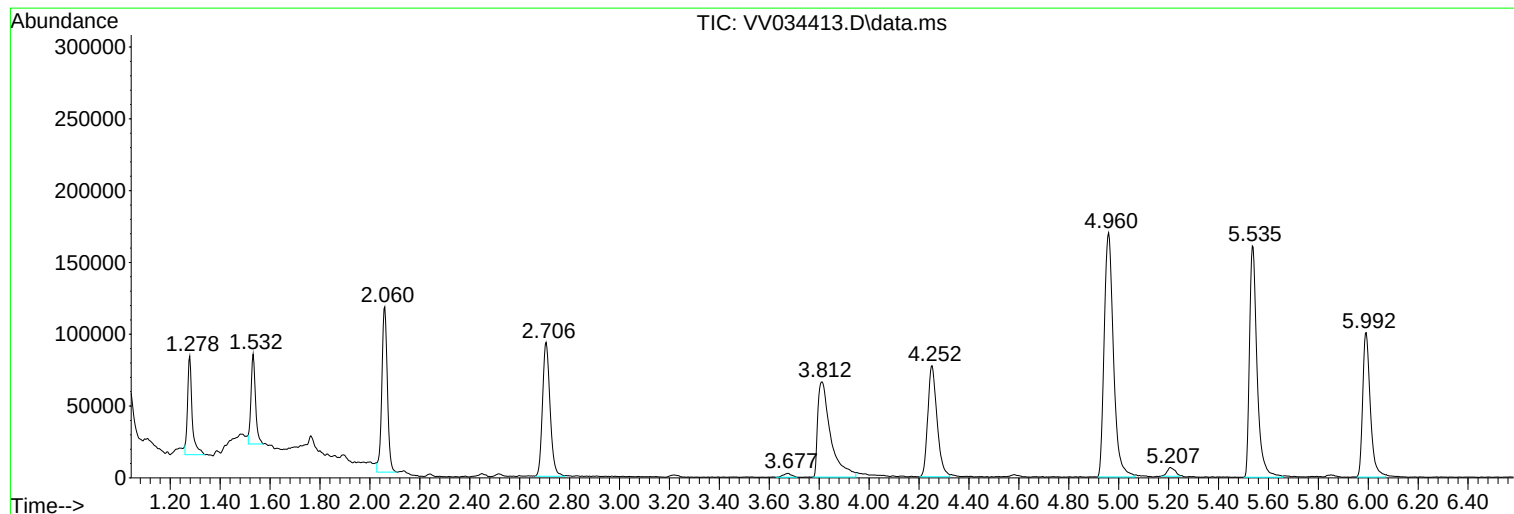

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022624\
Data File : VV034413.D
Acq On : 26 Feb 2024 17:30
Operator : SY/MD
Sample : P1503-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022624\
Data File : VV034413.D
Acq On : 26 Feb 2024 17:30
Operator : SY/MD
Sample : P1503-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc