

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022624\
 Data File : VV034427.D
 Acq On : 26 Feb 2024 23:07
 Operator : SY/MD
 Sample : P1535-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	94	rVB	57624	67168	13.73%	1.670%
2	1.532	146	153	171	rVB	53675	66678	13.63%	1.657%
3	2.060	307	317	331	rBV	98119	145982	29.84%	3.629%
4	2.706	505	518	532	rBV4	7450	16314	3.33%	0.406%
5	3.812	851	862	897	rBV3	76147	247211	50.53%	6.145%
6	4.252	984	999	1028	rBV	68205	181681	37.14%	4.516%
7	4.960	1204	1219	1253	rBV2	153859	396195	80.99%	9.848%
8	5.535	1388	1398	1425	rBV	151805	316366	64.67%	7.864%
9	5.838	1480	1492	1525	rBV	107839	225186	46.03%	5.597%
10	5.992	1525	1540	1563	rBV	90335	190204	38.88%	4.728%
11	6.921	1819	1829	1848	rBV2	37203	74366	15.20%	1.848%
12	7.246	1919	1930	1955	rBV	175372	314319	64.25%	7.813%
13	7.564	2017	2029	2047	rBV	21102	42020	8.59%	1.044%
14	7.908	2128	2136	2150	rVB3	15245	27865	5.70%	0.693%
15	8.027	2164	2173	2211	rBV	270619	489205	100.00%	12.160%
16	8.786	2398	2409	2436	rBV	237629	391016	79.93%	9.719%
17	10.156	2819	2835	2857	rBV2	75775	120444	24.62%	2.994%
18	10.329	2881	2889	2898	rVB2	5149	7483	1.53%	0.186%
19	11.188	3145	3156	3178	rBV	249245	388932	79.50%	9.667%
20	11.561	3261	3272	3294	rBV	191657	314480	64.28%	7.817%




Sum of corrected areas: 4023115

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022624\
Data File : VV034427.D
Acq On : 26 Feb 2024 23:07
Operator : SY/MD
Sample : P1535-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

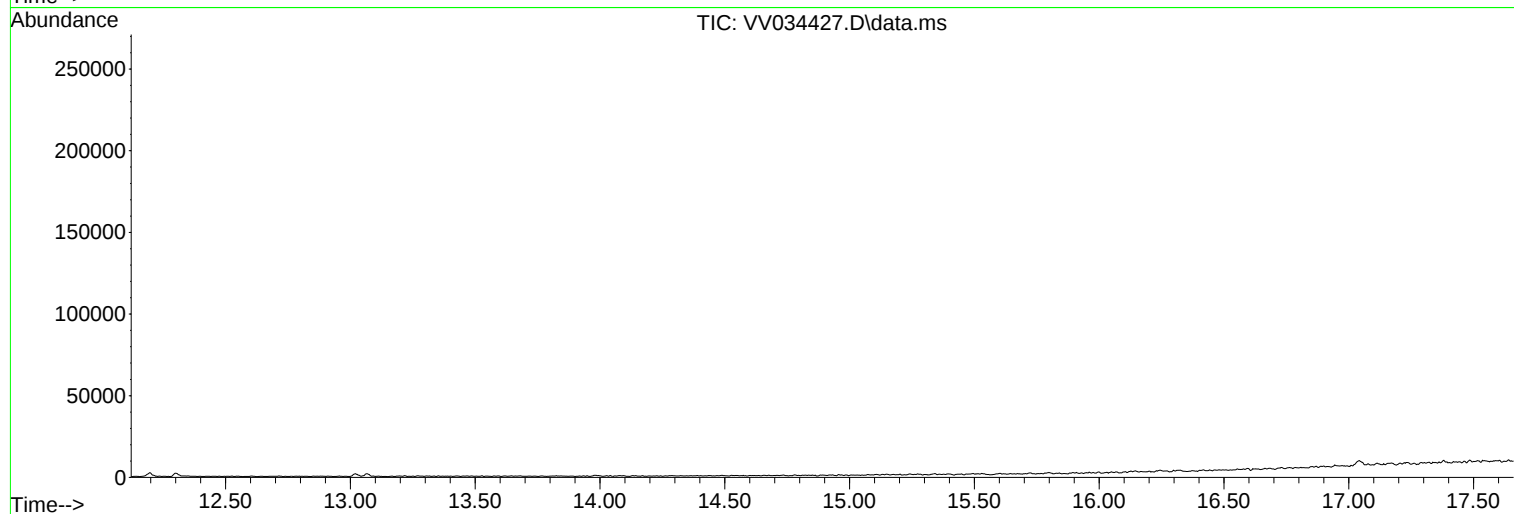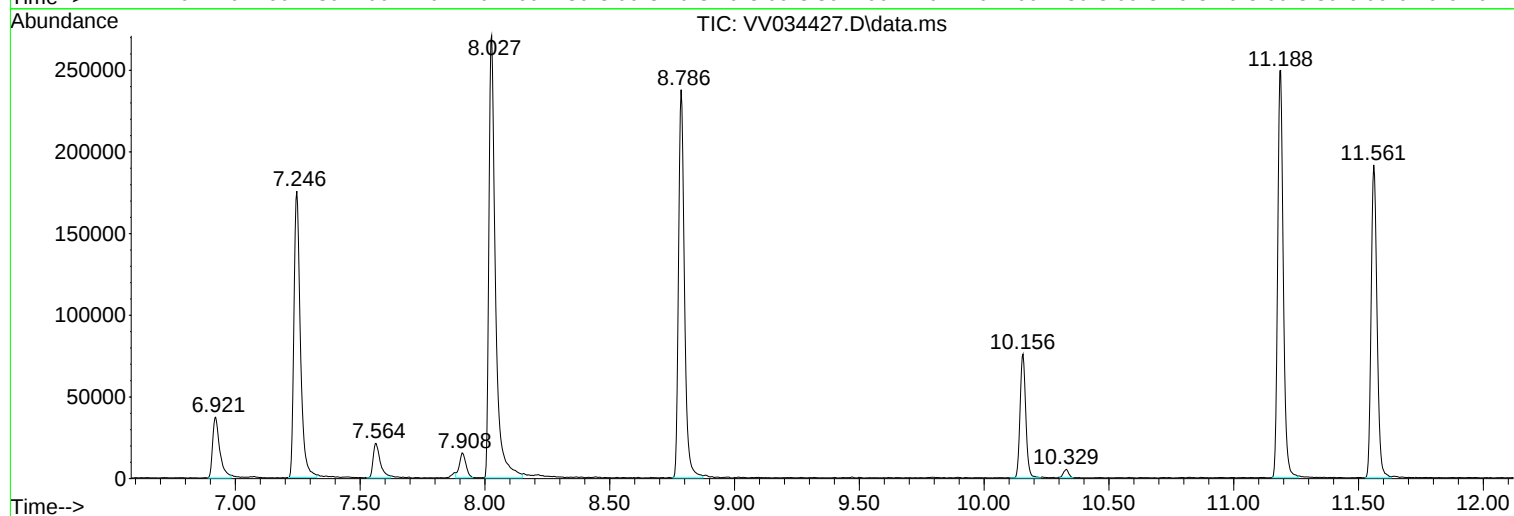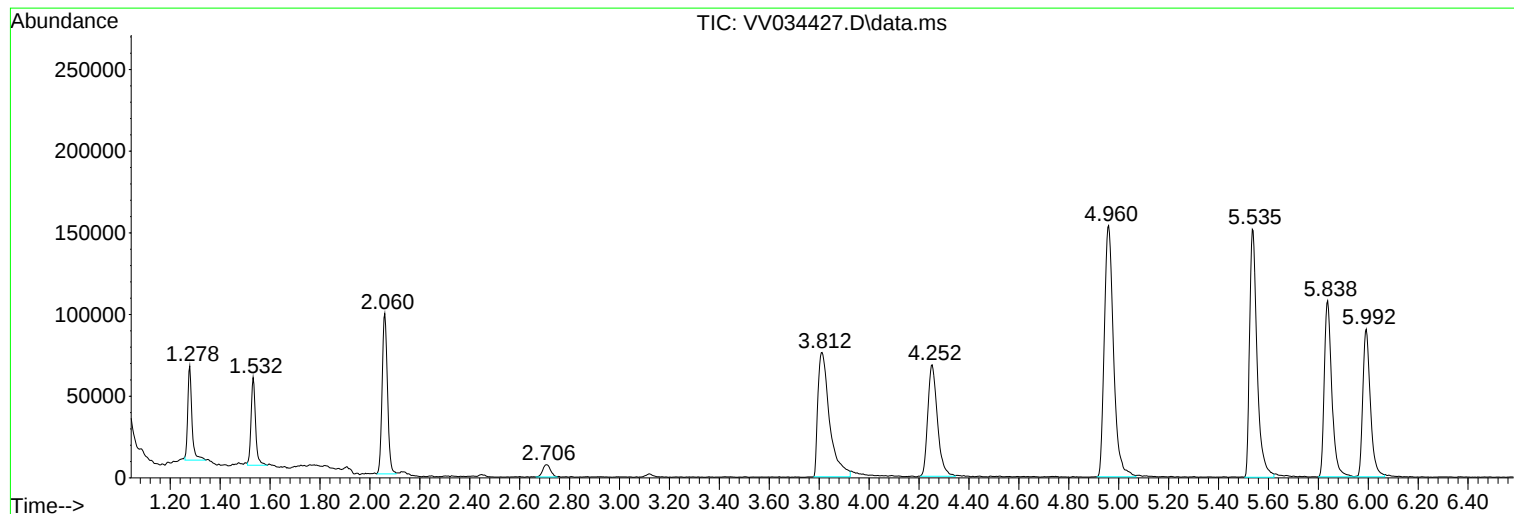

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022624\
Data File : VV034427.D
Acq On : 26 Feb 2024 23:07
Operator : SY/MD
Sample : P1535-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022624\
Data File : VV034427.D
Acq On : 26 Feb 2024 23:07
Operator : SY/MD
Sample : P1535-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc