


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022719\
 Data File : VV009389.D
 Acq On : 27 Feb 2019 10:06
 Operator : SY/MD
 Sample : BFB68
 Misc : 5.00G/10ML/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB68

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM022619S.M
 Title : VOC Analysis
 Last Update : Thu Feb 28 04:32:57 2019

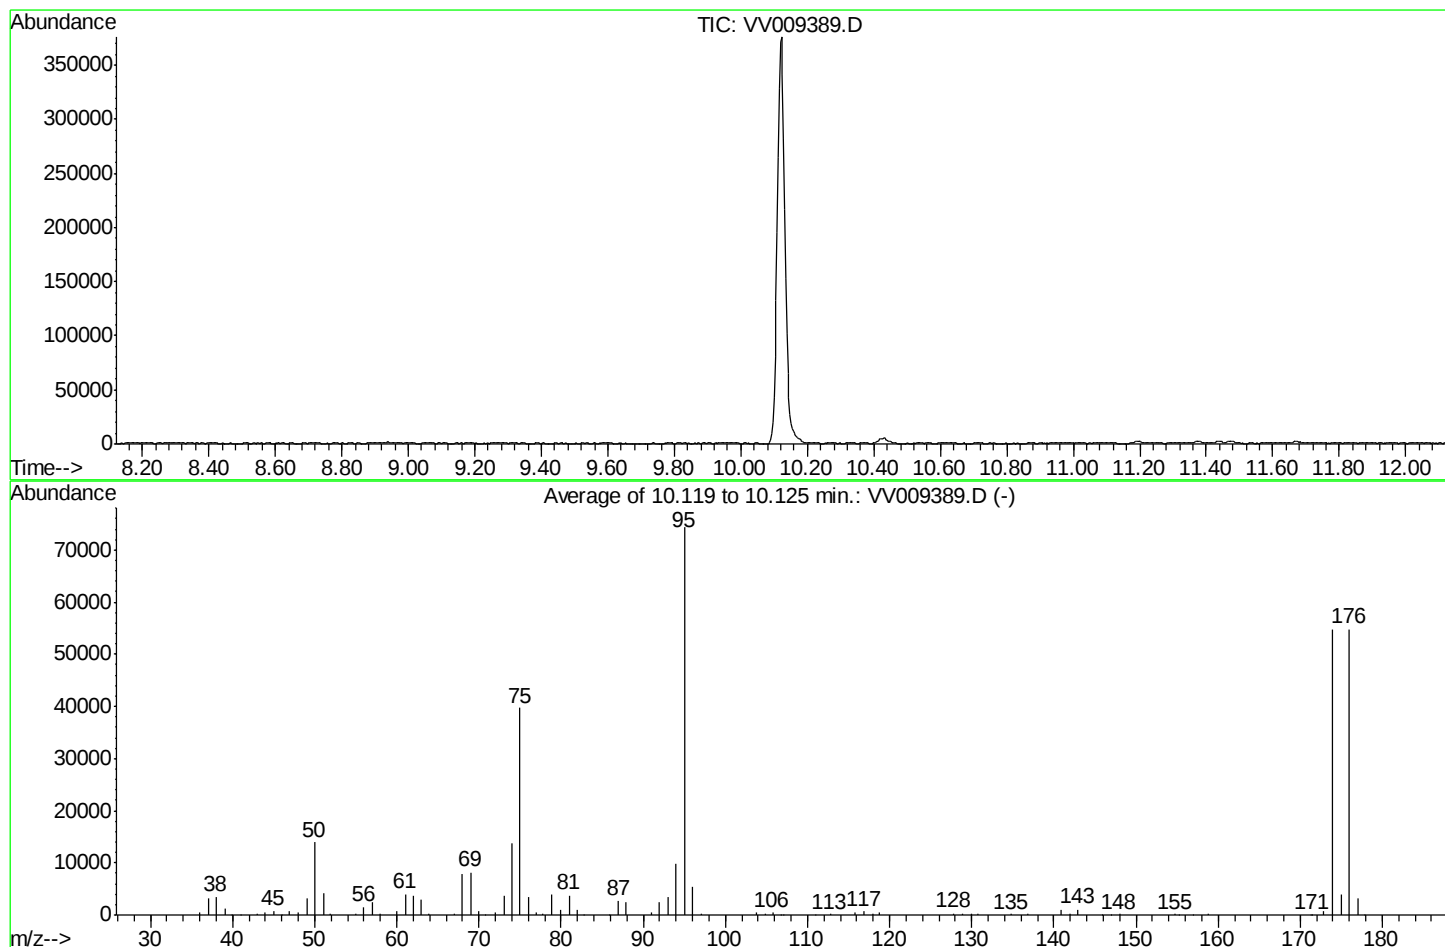

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	13935	PASS
75	95	30	80	53.5	39744	PASS
95	95	100	100	100.0	74346	PASS
96	95	5	9	7.2	5321	PASS
173	174	0.00	2	1.5	809	PASS
174	95	50	120	73.5	54672	PASS
175	174	5	9	7.3	3983	PASS
176	174	95	101	100.1	54744	PASS
177	176	5	9	5.9	3214	PASS

m/z	Abundance
35.90	642.0
37.00	3176.0
38.00	3588.0
39.00	1237.0
40.00	116.0
40.90	135.0
43.00	160.0
44.00	1021.0
45.00	796.0
45.90	122.0
46.90	748.0
48.10	511.0
49.00	3313.0
50.00	14568.0
51.10	4407.0
52.00	234.0
55.00	261.0
56.00	1553.0
57.10	2439.0
57.90	186.0
59.90	726.0
61.00	4080.0
62.10	3814.0
63.00	2954.0
63.90	281.0
67.10	217.0
68.00	7970.0
69.00	8057.0
70.00	768.0
70.70	110.0
71.90	437.0
73.00	3836.0
74.00	14035.0
75.00	40944.0
76.00	3415.0
76.90	464.0
77.80	329.0
78.90	4000.0
79.90	916.0
81.00	3784.0
81.90	963.0
82.80	119.0
85.90	133.0
87.00	2724.0
88.00	2697.0
91.00	410.0
92.00	2396.0
93.00	3543.0
94.00	10230.0
95.00	75864.0
96.00	5346.0
97.00	128.0
103.80	409.0
104.90	144.0
105.80	423.0
106.80	101.0
111.00	114.0
112.70	173.0
115.80	422.0
116.90	665.0
117.90	348.0
118.80	514.0
127.80	284.0
128.90	150.0
129.90	263.0
130.80	141.0
134.80	168.0
136.80	126.0
140.90	964.0
142.00	131.0
143.00	1143.0
145.80	107.0
148.00	139.0
154.80	186.0
157.00	114.0
158.80	153.0
172.90	829.0
174.00	55912.0
175.00	4143.0
176.00	55320.0
177.00	3363.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
35.90	624.0
37.00	3275.0
38.00	3580.0
39.00	1203.0
39.90	100.0
40.90	101.0
43.00	152.0
44.00	1005.0
45.00	793.0
46.90	763.0
48.00	496.0
49.00	3329.0
50.00	14364.0
51.10	4311.0
51.90	238.0
55.00	272.0
56.00	1543.0
57.00	2502.0
57.90	224.0
59.90	658.0
61.00	4099.0
62.00	3742.0
63.00	2893.0
63.90	296.0
67.00	227.0
68.00	7967.0
69.00	8382.0
70.00	710.0
70.70	131.0
72.00	441.0
73.00	3922.0
74.00	14185.0
75.00	41320.0
76.00	3443.0
76.90	401.0
77.70	342.0
78.90	3938.0
80.00	866.0
80.90	3898.0
81.90	959.0
85.90	142.0
87.00	2887.0
87.90	2614.0
90.90	414.0
92.00	2433.0
93.00	3514.0
94.00	10271.0
95.00	77256.0
96.00	5530.0
97.00	135.0
103.80	429.0
104.90	181.0
105.80	468.0
112.80	162.0
115.80	432.0
116.90	679.0
117.90	341.0
118.80	479.0
127.80	308.0
128.90	145.0
129.90	272.0
130.80	157.0
134.80	160.0
136.80	142.0
140.90	1067.0
142.00	153.0
142.90	1156.0
145.80	139.0
148.00	151.0
154.80	175.0
155.20	105.0
157.00	128.0
158.80	156.0
171.30	127.0
172.90	836.0
174.00	56528.0
175.00	4056.0
176.00	56736.0
177.00	3275.0
177.80	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
35.90	519.0
37.00	3106.0
38.00	3184.0
39.10	1128.0
39.90	103.0
43.00	167.0
44.00	870.0
45.00	718.0
47.00	691.0
48.00	405.0
49.00	2900.0
50.00	12873.0
51.00	3914.0
51.90	215.0
55.00	254.0
56.00	1367.0
57.00	2329.0
57.90	197.0
60.00	548.0
61.00	3649.0
62.00	3370.0
63.00	2679.0
63.90	271.0
66.90	221.0
68.00	7311.0
69.00	7939.0
69.90	577.0
70.70	125.0
72.00	412.0
73.00	3485.0
74.00	12715.0
75.00	36968.0
76.00	3204.0
76.90	298.0
77.70	283.0
78.90	3519.0
80.00	865.0
80.90	3682.0
81.90	902.0
87.00	2776.0
87.90	2295.0
90.90	371.0
92.00	2236.0
93.00	3079.0
94.00	9303.0
95.00	69920.0
96.00	5089.0
97.10	155.0
103.80	389.0
104.90	192.0
105.80	437.0
107.00	122.0
112.80	122.0
115.90	365.0
116.90	604.0
117.90	326.0
118.80	423.0
127.90	284.0
128.80	130.0
129.90	280.0
130.80	135.0
134.90	128.0
136.80	175.0
140.90	1070.0
142.00	144.0
142.90	1012.0
145.90	137.0
146.90	109.0
148.00	121.0
154.80	155.0
156.90	124.0
158.80	112.0
171.50	141.0
172.90	763.0
174.00	51576.0
175.00	3751.0
176.00	52176.0
177.00	3004.0
177.80	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
44.00	447.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68