

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022721\
 Data File : VW020409.D
 Acq On : 26 Feb 2021 12:29
 Operator : SY/MD
 Sample : M1513-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG0L9

Manual Integrations
 APPROVED

MMDadoda
 3/1/2021 10:01:16 AM

Quant Time: Feb 27 01:12:12 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Feb 27 01:11:28 2021
 Response via : Initial Calibration

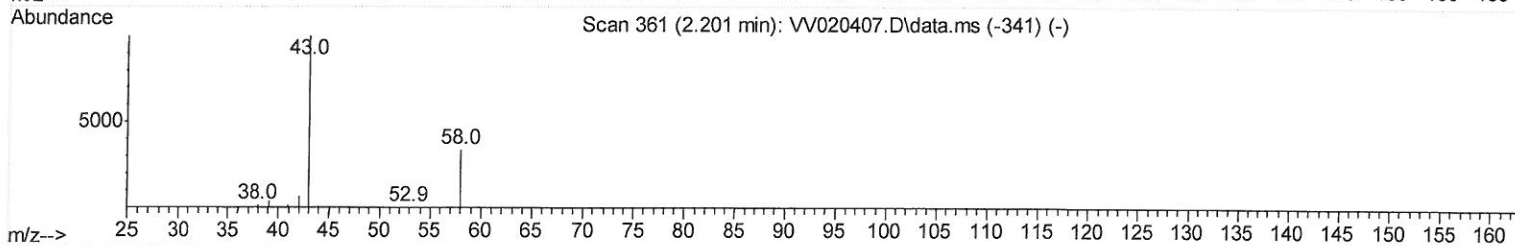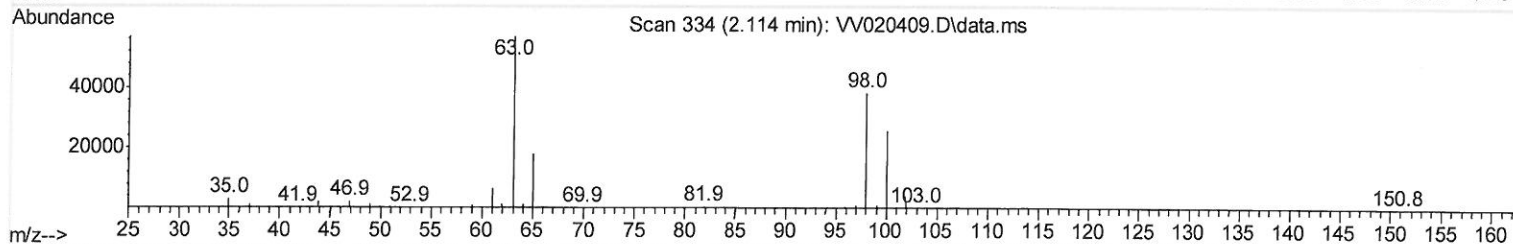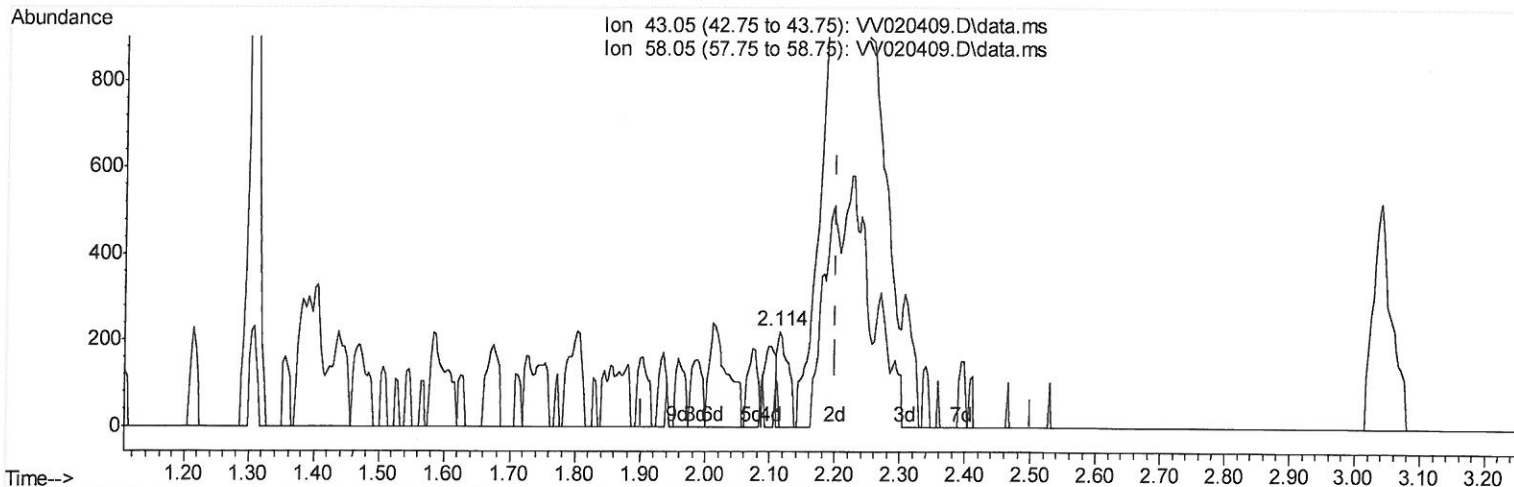

TIC: VW020409.D\data.ms

(13) Acetone (T)

2.114min (-0.087) 0.07 ug/L

response 255

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	9.30	16.08
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022721\
 Data File : VW020409.D
 Acq On : 26 Feb 2021 12:29
 Operator : SY/MD
 Sample : M1513-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG0L9

Manual Integrations
 APPROVED

MMDadoda
 3/1/2021 10:01:16 AM

Quant Time: Feb 27 01:12:12 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Feb 27 01:11:28 2021
 Response via : Initial Calibration

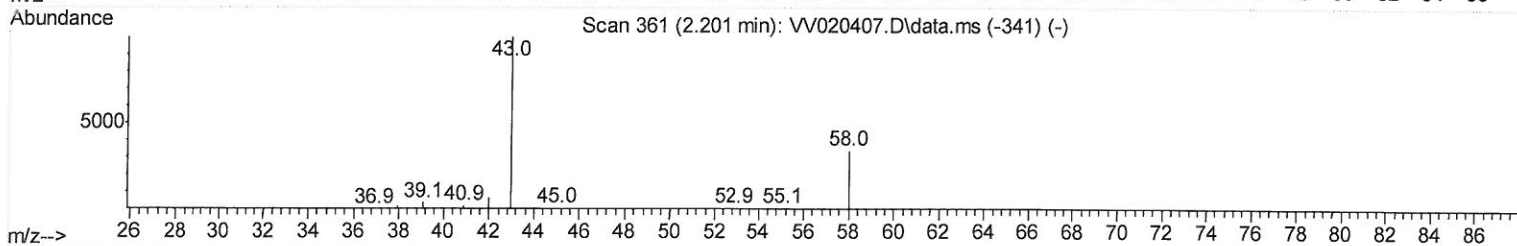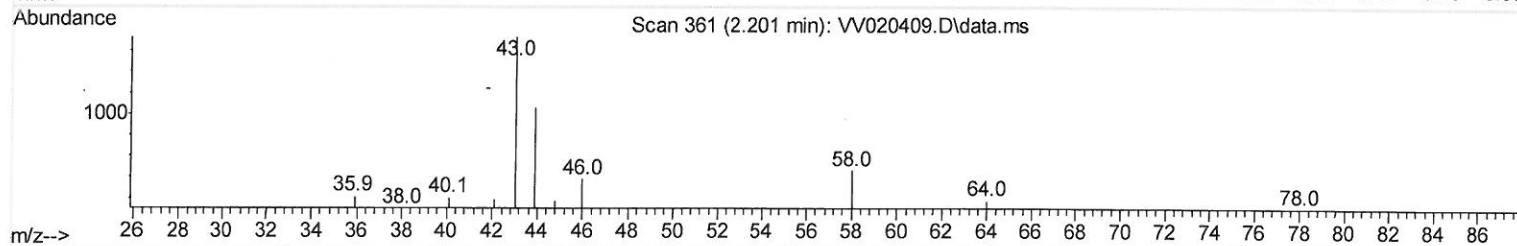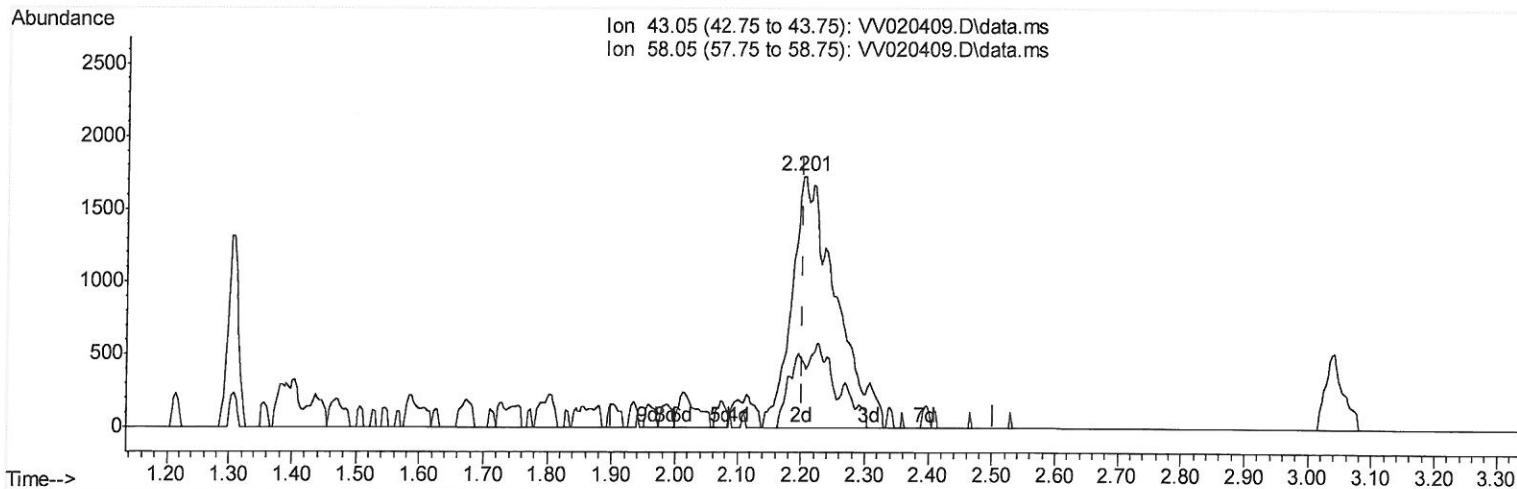

TIC: VW020409.D\data.ms

(13) Acetone (T)

2.201min (-0.000) 2.35 ug/L m

response 8310

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	9.30	0.49
0.00	0.00	0.00
0.00	0.00	0.00

263/01/21 Sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\W022721\
 Data File : W020409.D
 Acq On : 26 Feb 2021 12:29
 Operator : SY/MD
 Sample : M1513-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG0L9

Manual Integrations
 APPROVED

MMDadoda
 3/1/2021 10:01:16 AM

Quant Time: Feb 27 01:12:12 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Feb 27 01:11:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	320179	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	307988	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.255	152	146511	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	106302	4.71	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	94.20%	
7) Chloroethane-d5	1.564	69	81849	4.62	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	92.40%	
11) 1,1-Dichloroethene-d2	2.105	63	136671	3.11	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	62.20%	
20) 2-Butanone-d5	3.912	46	151571	38.81	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	77.62%	
24) Chloroform-d	4.349	84	170973	4.24	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	84.80%	
26) 1,2-Dichloroethane-d4	5.034	65	83762	4.27	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.40%	
32) Benzene-d6	5.050	84	352831	4.57	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.40%	
36) 1,2-Dichloropropane-d6	6.069	67	101630	4.45	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	89.00%	
41) Toluene-d8	7.317	98	317082	4.26	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.20%	
45) trans-1,3-Dichloroprop...	7.625	79	33012	3.78	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	75.60%	
48) 2-Hexanone-d5	8.095	63	99703	32.58	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	65.16%	
59) 1,1,2,2-Tetrachloroeth...	10.223	84	55203	3.40	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	68.00%	
65) 1,2-Dichlorobenzene-d4	11.632	152	125375	4.82	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.40%	
Target Compounds						
13) Acetone	2.201	43	8310m	2.35	ug/L	Qvalue 91
16) Methylene chloride	2.507	84	5756	0.20	ug/L	91
25) Chloroform	4.378	83	6453	0.12	ug/L	85
50) 2-Hexanone	8.146	43	16799	1.82	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022721\
Data File : VW020409.D
Acq On : 26 Feb 2021 12:29
Operator : SY/MD
Sample : M1513-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG0L9

Manual Integrations
APPROVED

MMDadoda
3/1/2021 10:01:16 AM

Quant Time: Feb 27 01:12:12 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Feb 27 01:11:28 2021
Response via : Initial Calibration

