
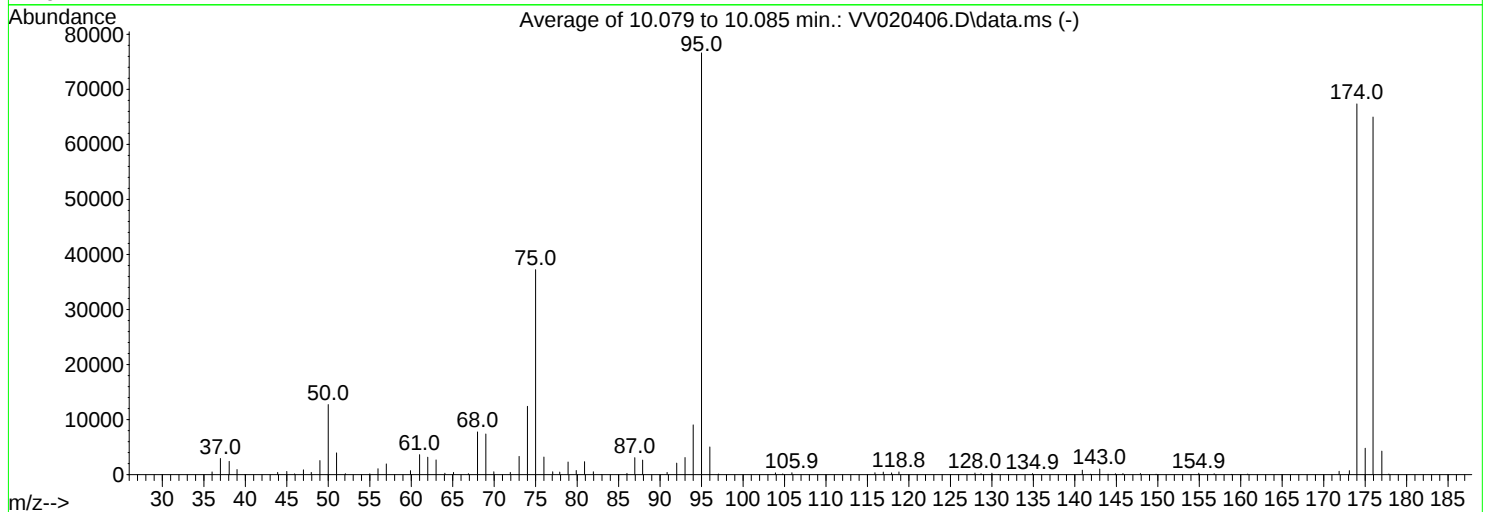


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022721\
 Data File : VV020406.D
 Acq On : 26 Feb 2021 09:21
 Operator : SY/MD
 Sample : BFB33
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB33

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVTR022221WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Feb 27 01:11:28 2021

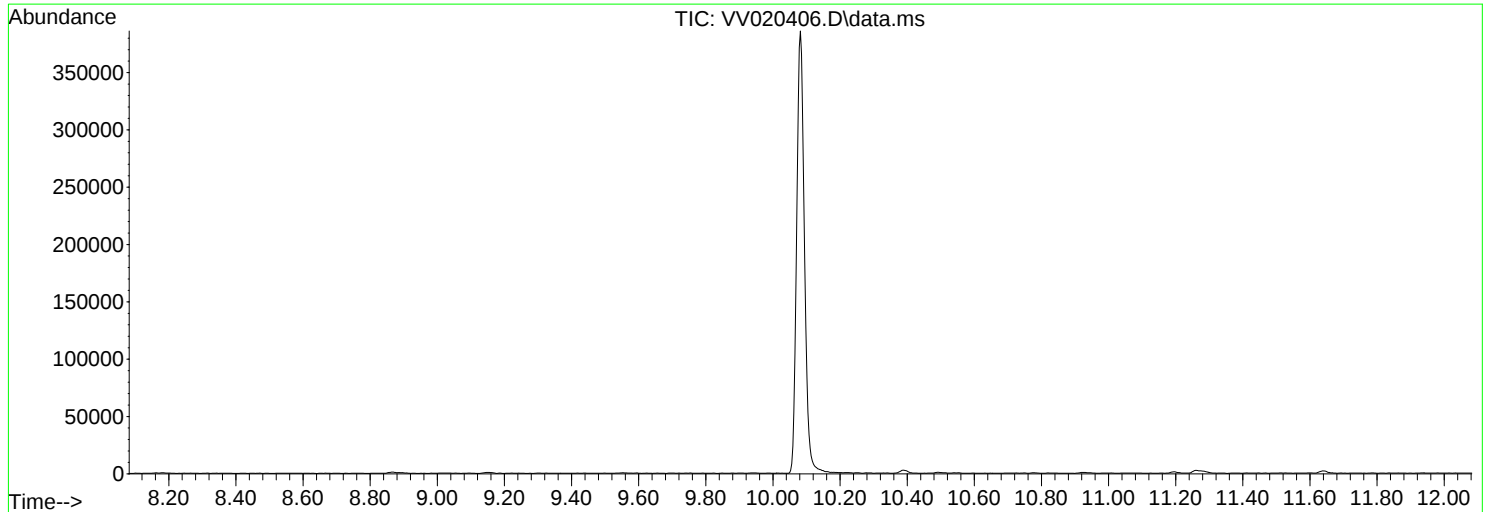

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	12733	PASS
75	95	30	80	48.6	37240	PASS
95	95	100	100	100.0	76632	PASS
96	95	5	9	6.6	5021	PASS
173	174	0.00	2	1.1	742	PASS
174	95	50	120	87.9	67363	PASS
175	174	5	9	7.1	4794	PASS
176	174	95	101	96.5	64973	PASS
177	176	5	9	6.6	4282	PASS

m/z	Abundance
40.00	142.0
43.90	378.0

Instrument :
MSVOA_V
ClientSampleId :
BFB33

m/z	Abundance
36.00	454.0
37.00	3068.0
38.10	2418.0
39.00	943.0
39.90	150.0
44.00	727.0
45.00	603.0
45.90	169.0
47.00	941.0
47.90	480.0
49.00	2557.0
50.00	12909.0
51.00	4036.0
52.10	204.0
55.00	164.0
56.00	1063.0
57.00	2063.0
59.90	761.0
61.00	3570.0
62.00	3216.0
63.00	2786.0
64.00	287.0
65.10	401.0
66.90	152.0
68.00	8117.0
69.00	7319.0
70.00	527.0
72.00	462.0
73.00	3233.0
74.00	12395.0
75.00	37352.0
76.00	3312.0
77.10	527.0
77.90	392.0
78.90	2296.0
79.90	758.0
80.90	2223.0
82.00	535.0
86.00	269.0
87.00	3018.0
87.90	2681.0
90.90	366.0
92.00	2128.0
93.00	3154.0
94.00	9071.0
95.00	76496.0
96.00	5005.0
97.00	177.0
103.90	338.0
104.80	137.0
105.90	317.0
115.90	362.0
116.90	494.0
117.90	314.0
118.80	521.0
128.00	302.0
128.70	163.0
130.00	279.0
130.80	111.0
134.90	176.0
140.90	832.0
141.90	147.0
143.00	1055.0
144.00	123.0
144.80	138.0
145.80	176.0
147.90	176.0
149.80	114.0
155.00	247.0
156.70	162.0
160.80	108.0
171.90	582.0
173.10	685.0
174.00	65656.0
175.00	4620.0
176.00	63232.0
177.00	4150.0
177.90	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB33

m/z	Abundance
36.00	508.0
37.00	3027.0
38.00	2467.0
39.00	980.0
39.90	146.0
43.90	831.0
45.00	611.0
46.00	158.0
47.00	899.0
47.90	402.0
49.00	2648.0
50.00	13153.0
51.00	4065.0
52.00	171.0
55.00	144.0
56.00	1103.0
57.00	2013.0
59.90	783.0
61.00	3792.0
62.00	3290.0
63.00	2764.0
64.00	271.0
65.20	427.0
66.90	187.0
68.00	8074.0
69.00	7605.0
69.90	544.0
71.90	434.0
73.00	3445.0
74.00	12722.0
75.00	38424.0
76.00	3243.0
77.00	563.0
77.90	481.0
78.90	2332.0
79.90	753.0
80.90	2416.0
81.90	533.0
86.00	231.0
87.00	3161.0
87.90	2718.0
90.80	453.0
92.00	2117.0
93.00	3188.0
94.00	9406.0
95.00	78824.0
96.00	5131.0
97.10	139.0
103.90	344.0
104.80	168.0
105.90	376.0
115.90	362.0
116.90	465.0
117.90	346.0
118.80	529.0
128.00	315.0
128.70	197.0
130.00	278.0
134.90	213.0
140.90	823.0
141.90	141.0
143.00	1084.0
144.00	116.0
144.90	184.0
145.80	236.0
147.90	210.0
149.80	123.0
155.00	270.0
156.80	166.0
158.90	102.0
160.90	107.0
171.90	609.0
173.10	775.0
174.00	69392.0
175.00	4973.0
176.00	67080.0
177.00	4388.0
177.90	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB33

m/z	Abundance
36.00	568.0
37.00	2705.0
38.00	2360.0
39.00	905.0
40.00	149.0
43.90	828.0
45.00	521.0
46.00	146.0
47.00	777.0
48.00	340.0
49.00	2487.0
50.00	12138.0
51.00	3743.0
52.00	149.0
55.00	144.0
56.00	1039.0
57.00	1780.0
58.00	111.0
59.90	679.0
61.00	3530.0
62.00	3001.0
63.00	2492.0
64.10	276.0
65.00	369.0
66.90	223.0
68.00	7085.0
69.00	7274.0
69.90	505.0
71.90	343.0
73.00	3315.0
74.00	12109.0
75.00	35944.0
76.00	3084.0
77.00	510.0
77.90	504.0
78.90	2227.0
79.90	727.0
80.90	2427.0
81.90	513.0
82.90	116.0
86.00	182.0
86.90	3045.0
87.90	2572.0
90.80	408.0
92.00	2025.0
93.00	2961.0
94.00	8659.0
95.00	74576.0
96.00	4926.0
103.90	314.0
104.80	166.0
105.90	406.0
115.90	332.0
116.90	417.0
117.90	343.0
118.80	457.0
127.90	287.0
128.70	187.0
130.00	278.0
134.90	186.0
140.90	787.0
143.00	929.0
145.00	184.0
145.80	234.0
147.90	212.0
154.90	239.0
156.90	186.0
158.90	115.0
160.90	104.0
171.80	613.0
173.10	766.0
174.00	67040.0
175.00	4790.0
175.90	64608.0
177.00	4308.0
177.80	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB33