

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022819\
 Data File : VV009440.D
 Acq On : 28 Feb 2019 22:31
 Operator : SY/MD
 Sample : K1599-19
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CWK09

Quant Time: Mar 01 05:45:10 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Mar 01 03:49:54 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	97031	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	92146	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	42681	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	22981	4.54	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.80%
7) Chloroethane-d5	1.58	69	20626	4.50	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.00%
11) 1,1-Dichloroethene-d2	2.13	63	43942	3.43	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.60%
20) 2-Butanone-d5	3.96	46	49836	51.85	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.70%
24) Chloroform-d	4.40	84	47750	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.20%
26) 1,2-Dichloroethane-d4	5.09	65	24964	5.10	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.00%
32) Benzene-d6	5.10	84	97500	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.60%
36) 1,2-Dichloropropane-d6	6.12	67	30229	5.07	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.40%
41) Toluene-d8	7.36	98	96918	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
43) trans-1,3-Dichloropropene-	7.66	79	11740	4.45	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.00%
46) 2-Hexanone-d5	8.14	63	45662	53.38	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	106.76%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	22830	4.93	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	36286	5.29	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.80%


Target Compounds					Ovalue
13) Acetone	2.20	43	5201	5.696 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV022819\
Data File : VV009440.D
Acq On : 28 Feb 2019 22:31
Operator : SY/MD
Sample : K1599-19
Misc : 25ML/MSVOA V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CWK09

Quant Time: Mar 01 05:45:10 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Mar 01 03:49:54 2019
Response via : Initial Calibration

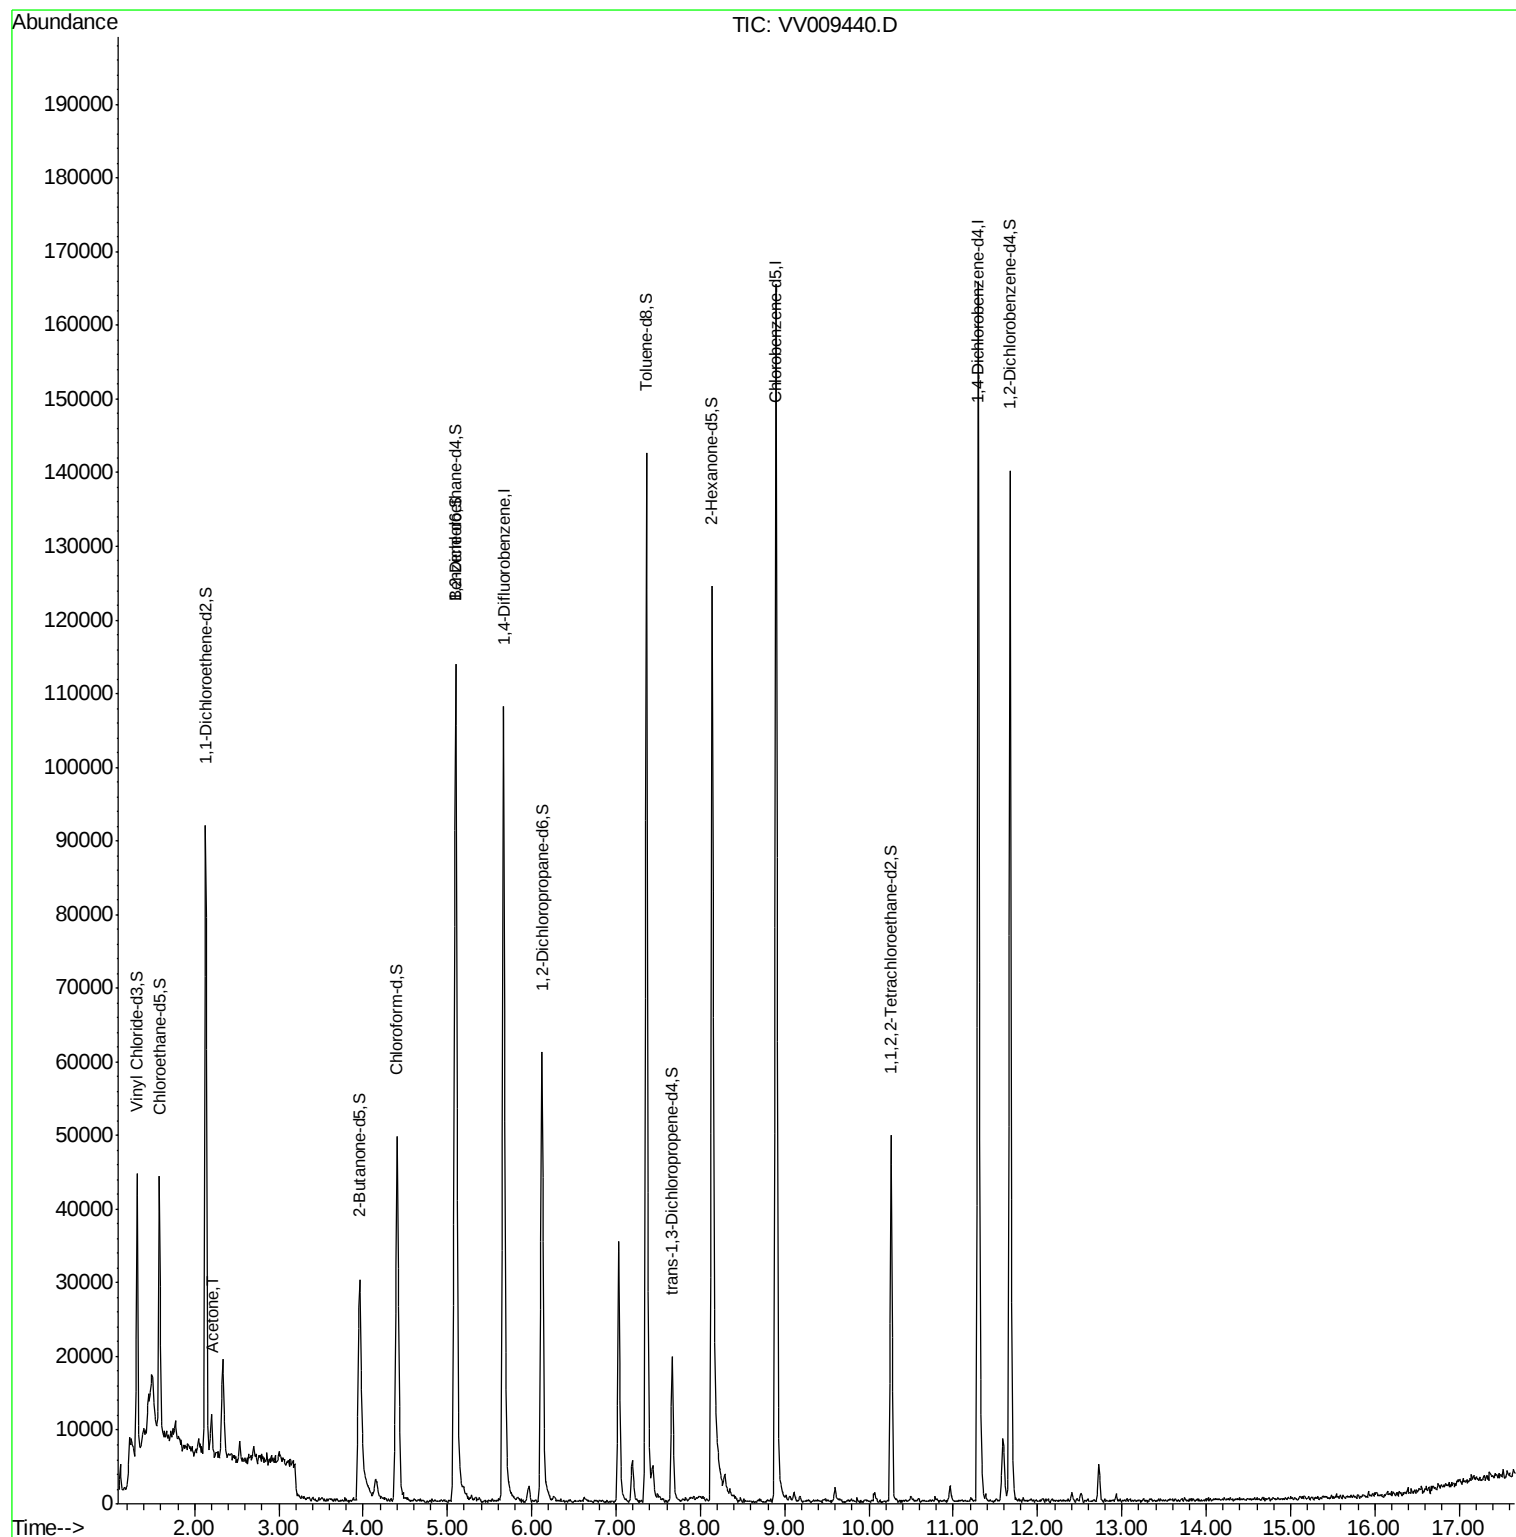

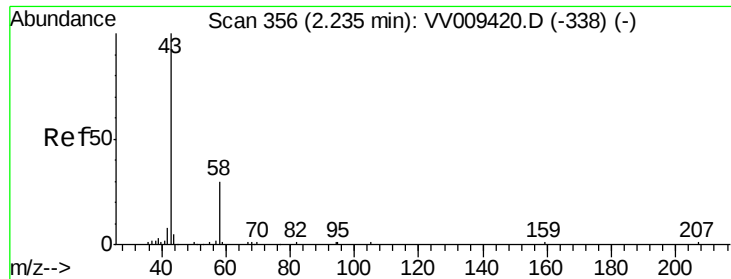

#13
 Acetone
 Concen: 5.696 ug/L
 RT: 2.20 min Scan# 345
 Delta R.T. -0.04 min
 Lab File: VV009440.D
 Acq: 28 Feb 2019 22:31

Instrument :
 MSVOA_V
 ClientSampleId :
 CWK09

Tot Ion: 43 Resp: 5201
 Ion Ratio Lower Upper
 43 100
 58 33.6 0.0 62.0

