

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022819\
 Data File : VV009441.D
 Acq On : 28 Feb 2019 22:57
 Operator : SY/MD
 Sample : K1599-20
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CWK12

Quant Time: Mar 01 05:47:14 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Mar 01 03:49:54 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	91588	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	88750	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	40414	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	22992	4.81	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.20%
7) Chloroethane-d5	1.58	69	21530	4.98	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.60%
11) 1,1-Dichloroethene-d2	2.13	63	44363	3.67	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.40%
20) 2-Butanone-d5	3.96	46	50716	55.91	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.82%
24) Chloroform-d	4.40	84	47132	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.60%
26) 1,2-Dichloroethane-d4	5.08	65	24661	5.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.80%
32) Benzene-d6	5.10	84	97625	5.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.40%
36) 1,2-Dichloropropane-d6	6.12	67	29061	5.07	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.40%
41) Toluene-d8	7.36	98	99253	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.00%
43) trans-1,3-Dichloropropene-	7.67	79	11606	4.57	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.40%
46) 2-Hexanone-d5	8.14	63	44730	54.29	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.58%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	23416	5.25	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	34848	5.36	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.20%


Target Compounds					Ovalue
13) Acetone	2.20	43	4410	5.117 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV022819\
Data File : VV009441.D
Acq On : 28 Feb 2019 22:57
Operator : SY/MD
Sample : K1599-20
Misc : 25ML/MSVOA V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CWK12

Quant Time: Mar 01 05:47:14 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Mar 01 03:49:54 2019
Response via : Initial Calibration

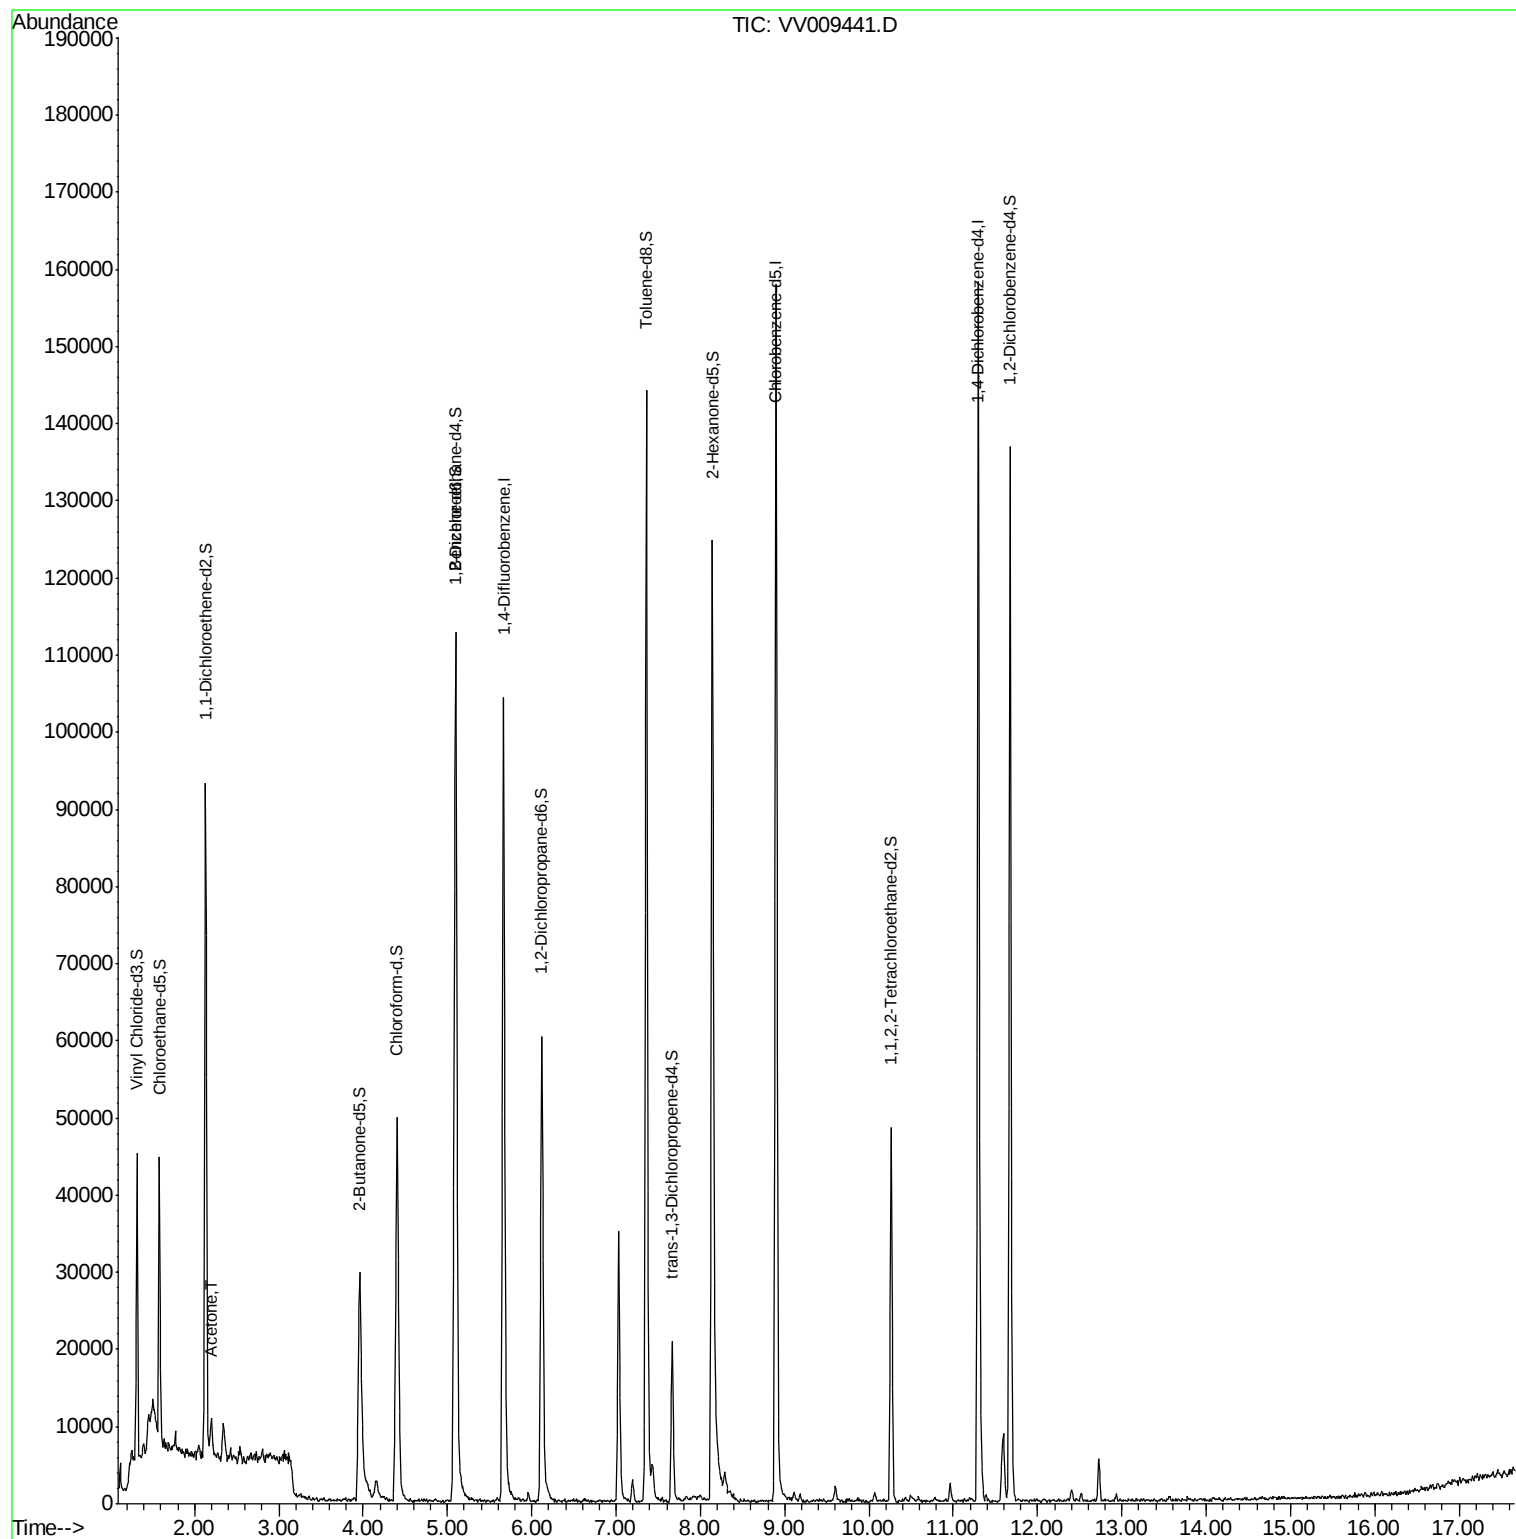

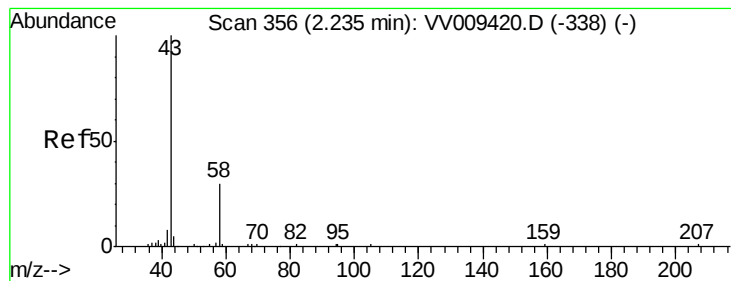

#13

Acetone

Concen: 5.117 ug/L

RT: 2.20 min Scan# 345

Delta R.T. -0.04 min

Lab File: VV009441.D

Acq: 28 Feb 2019 22:57

Instrument :
MSVOA_V
ClientSampleId :
CWK12

Tot Ion: 43 Resp: 4410

Ion Ratio Lower Upper

43 100

58 32.4 0.0 62.0

