

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022819\
 Data File : VV009434.D
 Acq On : 28 Feb 2019 19:57
 Operator : SY/MD
 Sample : K1599-13
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CWJZ7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022819WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.145	13	17	27	rVB	4938	4784	1.69%	0.178%
2	1.229	34	43	47	rBV3	2684	3972	1.40%	0.147%
3	1.319	60	71	81	rBV	39273	45687	16.13%	1.695%
4	1.489	112	124	138	rBV8	6450	16732	5.91%	0.621%
5	1.582	145	153	165	rBV	36011	44463	15.70%	1.650%
6	2.132	315	324	335	rBV	85847	121003	42.73%	4.490%
7	2.193	335	343	345	rBV7	3797	4299	1.52%	0.160%
8	2.328	376	385	399	rVB	22755	42550	15.02%	1.579%
9	3.232	655	666	674	rVB6	2291	3919	1.38%	0.145%
10	3.958	877	892	906	rBV2	40583	107719	38.04%	3.997%
11	4.405	1014	1031	1057	rBV2	49309	125321	44.25%	4.650%
12	5.097	1225	1246	1266	rBV3	114330	272478	96.21%	10.110%
13	5.666	1409	1423	1442	rBV	109664	222050	78.41%	8.239%
14	5.958	1504	1514	1529	rVB4	7288	13650	4.82%	0.506%
15	6.119	1550	1564	1583	rBV2	62219	128193	45.27%	4.757%
16	7.032	1835	1848	1865	rBV3	35811	65706	23.20%	2.438%
17	7.196	1888	1899	1909	rVB4	2876	5360	1.89%	0.199%
18	7.360	1937	1950	1965	rBV	143522	256863	90.70%	9.531%
19	7.431	1967	1972	1988	rVB	9629	17605	6.22%	0.653%
20	7.666	2033	2045	2067	rBV2	21418	37963	13.40%	1.409%
21	8.019	2146	2155	2165	rVB3	9767	16084	5.68%	0.597%
22	8.138	2180	2192	2231	rBV2	118945	262436	92.67%	9.738%
23	8.897	2416	2428	2448	rBV	168091	282657	99.81%	10.488%
24	10.264	2841	2853	2870	rBV	47404	75970	26.83%	2.819%
25	11.296	3163	3174	3201	rBV	164071	283201	100.00%	10.508%
26	11.582	3255	3263	3265	rBV2	3869	4732	1.67%	0.176%
27	11.675	3280	3292	3314	rVB	133688	229652	81.09%	8.521%


Sum of corrected areas: 2695049

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV022819\
Data File : VV009434.D
Acq On : 28 Feb 2019 19:57
Operator : SY/MD
Sample : K1599-13
Misc : 25ML/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CWJZ7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022819WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

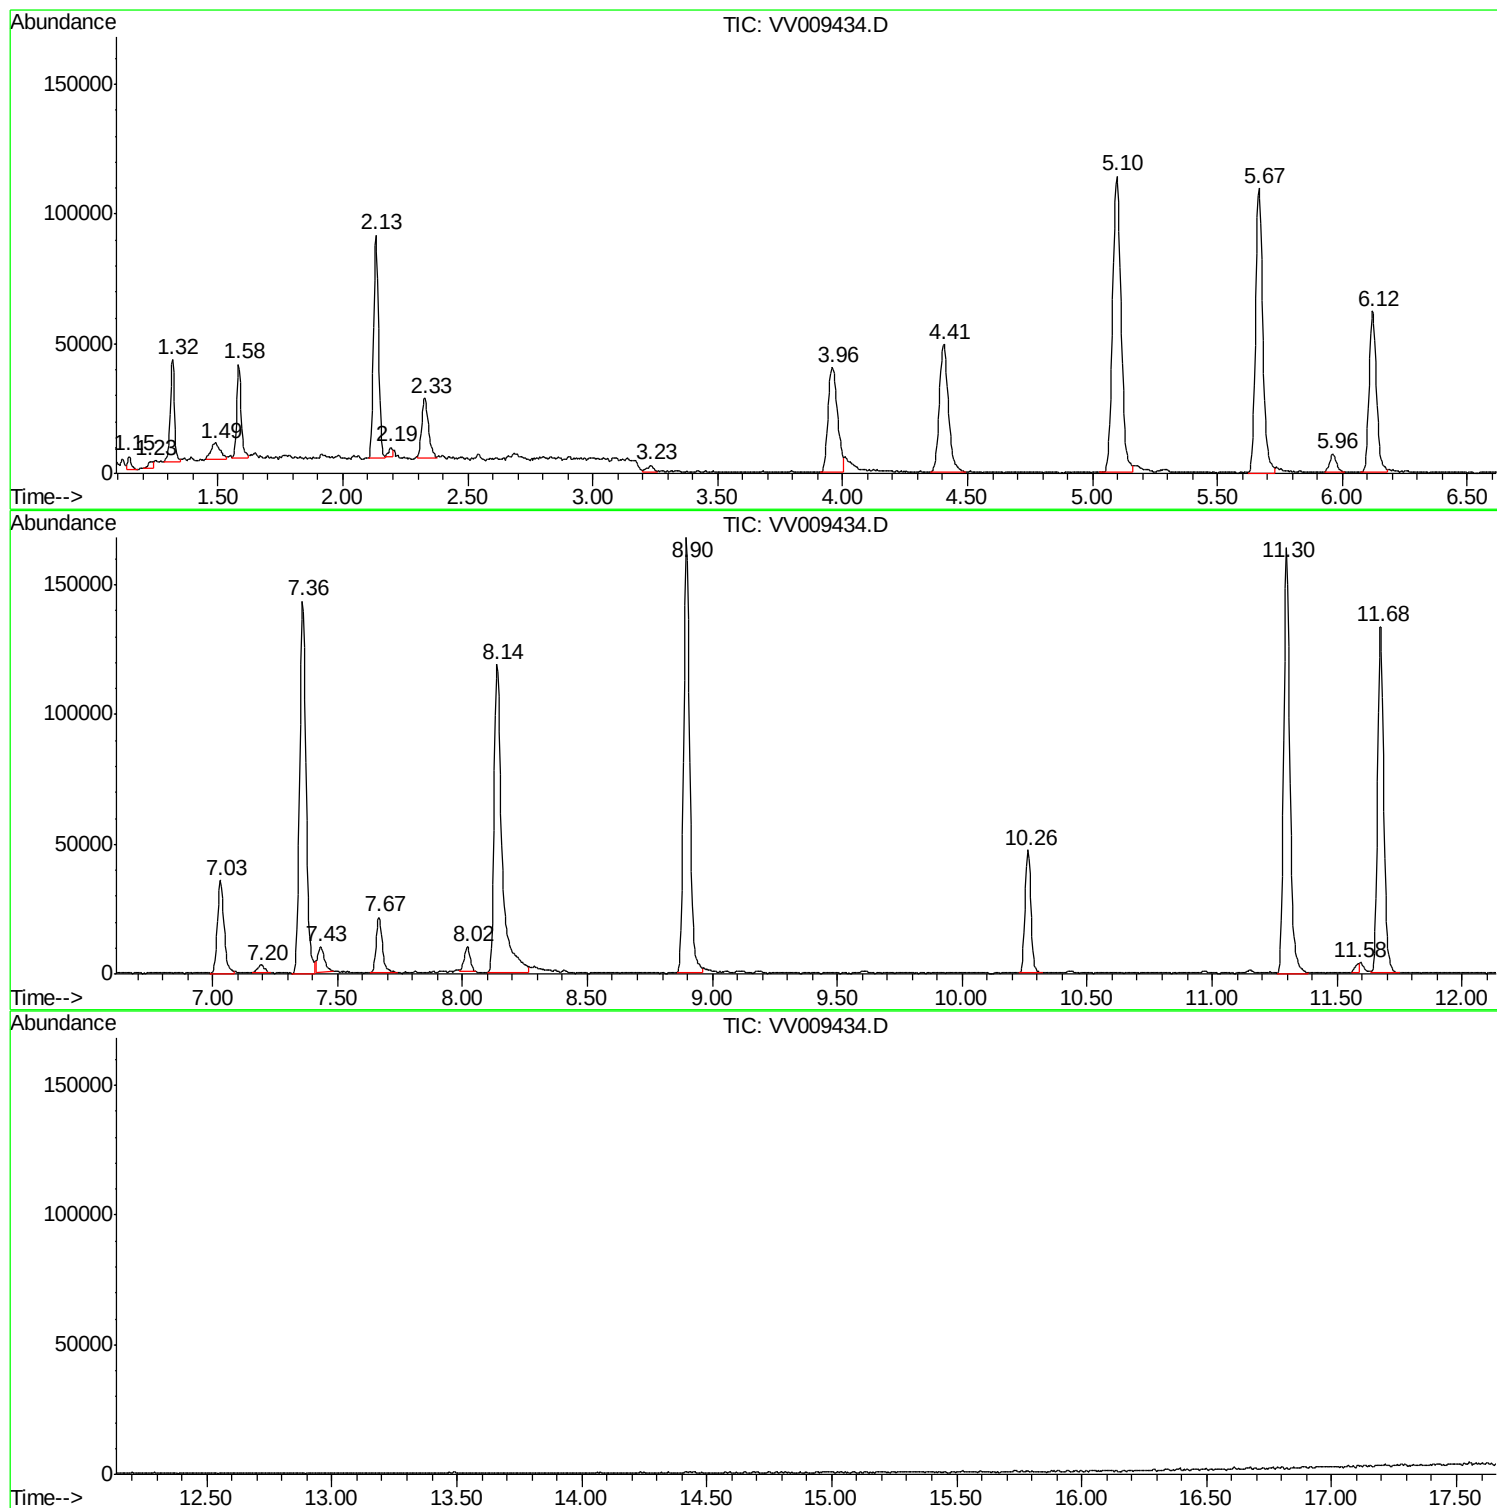

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV022819\
Data File : VV009434.D
Acq On : 28 Feb 2019 19:57
Operator : SY/MD
Sample : K1599-13
Misc : 25ML/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CWJZ7










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022819WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.33	0.96 ug/L	42550	1,4-Difluorobenzene	5.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	56
2		Isopropyl Alcohol	60	C3H8O	000067-63-0	56
3		R-(-)-1,2-propanediol	76	C3H8O2	004254-14-2	9
4		Propane, 2-ethoxy-	88	C5H12O	000625-54-7	9
5		2-Butanol, 3-methyl-	88	C5H12O	000598-75-4	9

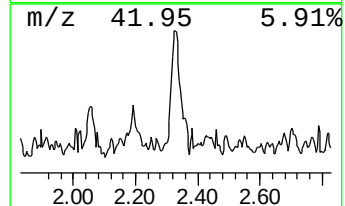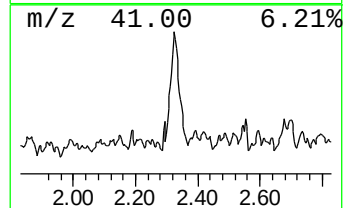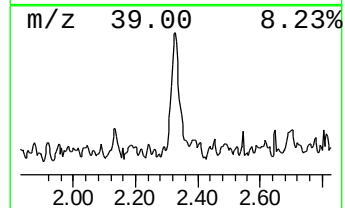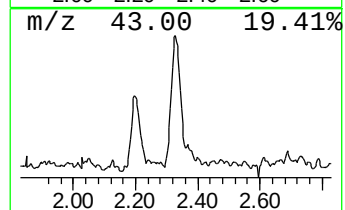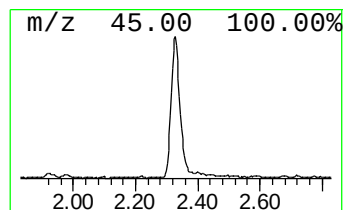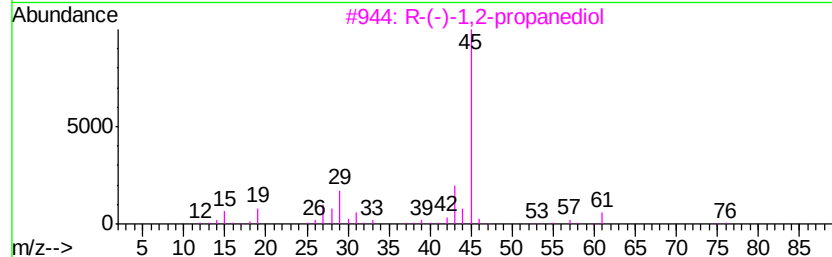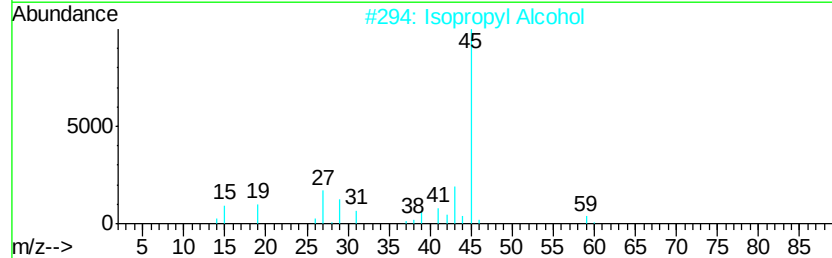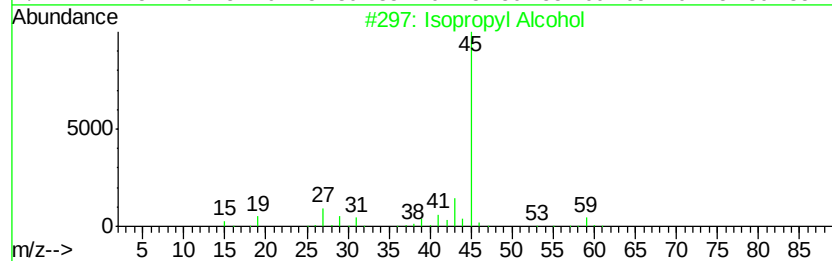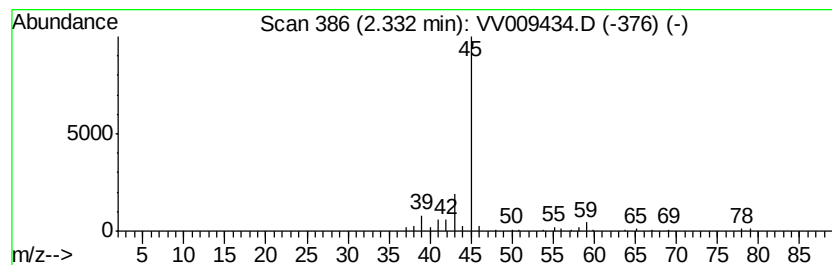

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV022819\
Data File : VV009434.D
Acq On : 28 Feb 2019 19:57
Operator : SY/MD
Sample : K1599-13
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CWJZ7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022819WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.33	1.0	ug/L	42550	1	5.67	222050	5.0