


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022819\
 Data File : VV009413.D
 Acq On : 28 Feb 2019 09:56
 Operator : SY/MD
 Sample : BFB69
 Misc : 25ML/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB69

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022819WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Mar 01 03:49:54 2019

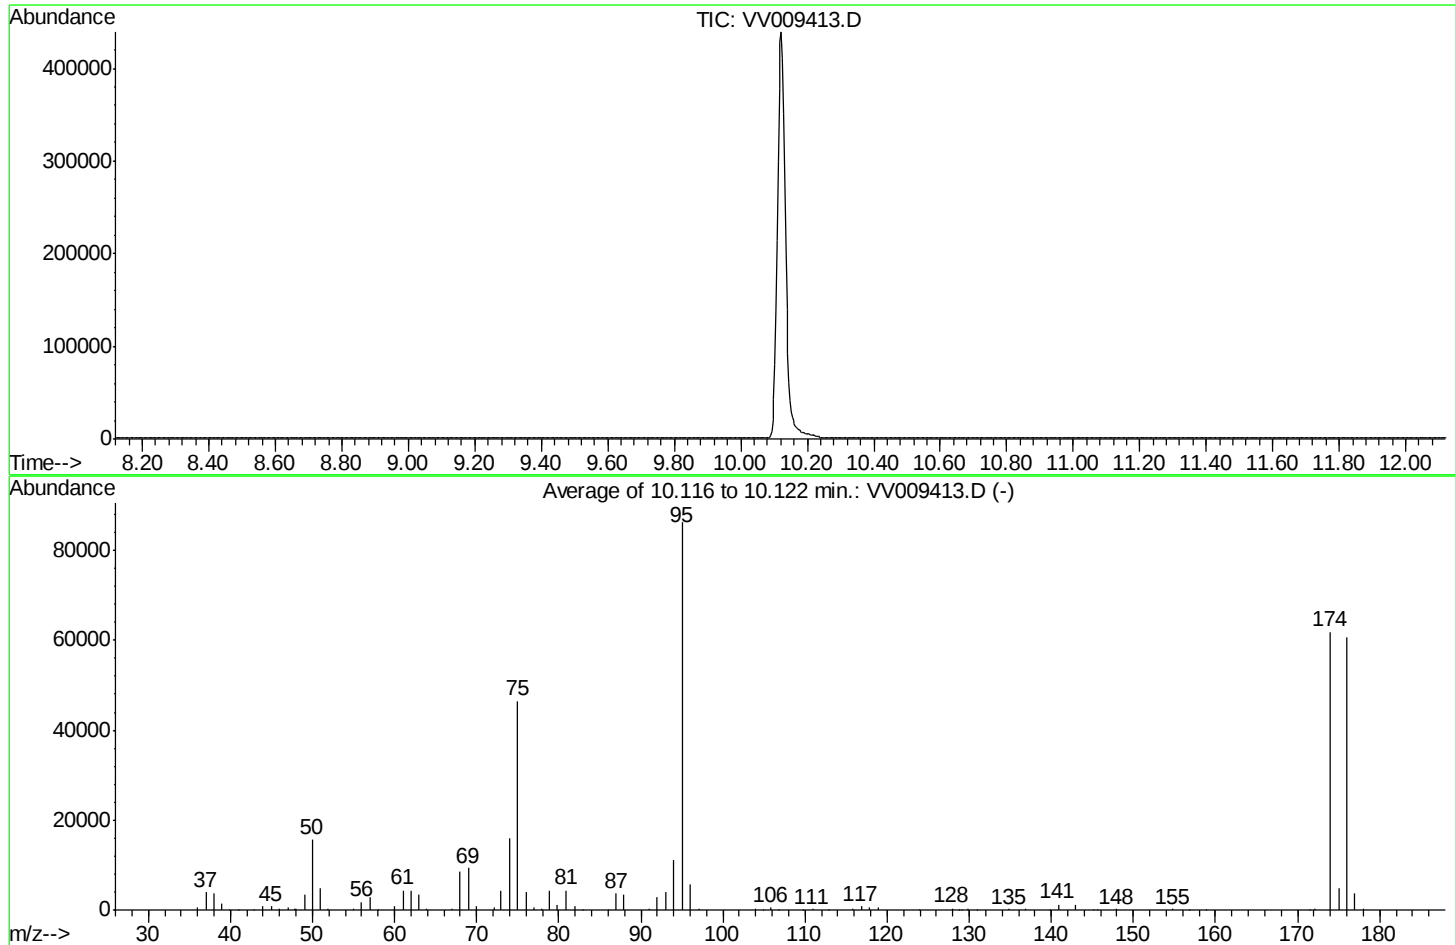

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	15580	PASS
75	95	30	80	53.9	46469	PASS
95	95	100	100	100.0	86248	PASS
96	95	5	9	6.5	5564	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.7	61821	PASS
175	174	5	9	7.9	4882	PASS
176	174	95	101	98.1	60677	PASS
177	176	5	9	6.1	3708	PASS

m/z	Abundance
36.00	481.0
37.00	3636.0
38.00	3479.0
39.00	1448.0
39.80	673.0
40.90	168.0
44.00	855.0
45.00	753.0
45.90	131.0
47.00	592.0
48.10	381.0
49.00	3343.0
50.00	14340.0
51.00	4634.0
51.90	178.0
55.00	253.0
56.00	1608.0
57.00	2487.0
57.90	131.0
60.00	752.0
61.00	3923.0
62.00	4026.0
63.00	3071.0
63.90	304.0
66.90	320.0
68.00	7875.0
69.00	8597.0
70.00	876.0
72.10	438.0
73.00	3873.0
74.00	14413.0
75.00	42360.0
76.00	3903.0
77.00	536.0
78.00	286.0
78.90	3932.0
79.80	997.0
80.90	4111.0
81.90	858.0
82.90	135.0
86.00	116.0
87.00	3367.0
87.90	3448.0
90.90	362.0
92.00	2761.0
93.00	3693.0
94.00	9989.0
95.00	80296.0
96.00	5145.0
97.10	238.0
103.90	325.0
104.90	145.0
105.90	513.0
111.00	170.0
112.80	135.0
115.90	293.0
116.90	713.0
117.90	418.0
119.00	457.0
124.00	102.0
128.00	294.0
128.70	132.0
129.10	118.0
129.80	313.0
134.90	149.0
136.80	170.0
139.70	112.0
140.90	1100.0
142.90	971.0
148.00	198.0
154.80	219.0
156.70	133.0
158.90	128.0
174.00	54488.0
175.00	4412.0
176.00	53680.0
177.00	3386.0
178.00	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

m/z	Abundance
36.00	565.0
37.00	4026.0
38.00	3884.0
39.00	1538.0
39.80	658.0
40.90	156.0
44.00	1024.0
45.00	832.0
45.90	208.0
47.00	749.0
48.00	405.0
49.00	3642.0
50.00	16134.0
51.00	5130.0
51.90	189.0
55.00	290.0
56.00	1860.0
57.00	2906.0
57.90	139.0
60.00	795.0
61.00	4424.0
62.00	4415.0
63.00	3404.0
63.90	331.0
67.00	320.0
68.00	8662.0
69.00	9692.0
70.00	843.0
72.10	493.0
73.00	4448.0
74.00	16488.0
75.00	48256.0
76.00	4151.0
77.10	491.0
78.00	333.0
78.90	4432.0
79.80	1079.0
80.90	4493.0
81.90	891.0
82.80	138.0
87.00	3805.0
88.00	3606.0
91.00	423.0
92.00	3052.0
93.00	4260.0
94.00	11397.0
95.00	89376.0
96.00	5628.0
97.10	258.0
103.90	412.0
104.90	144.0
105.80	573.0
106.80	130.0
111.00	165.0
112.80	128.0
115.80	315.0
116.90	843.0
117.90	504.0
119.00	426.0
124.00	118.0
127.90	358.0
128.80	142.0
129.90	347.0
131.00	135.0
134.90	173.0
136.90	231.0
139.80	115.0
140.90	1212.0
142.90	1148.0
145.10	106.0
145.60	125.0
147.90	240.0
154.80	259.0
156.70	126.0
158.90	158.0
172.10	251.0
174.00	63480.0
175.00	5069.0
176.00	62712.0
177.00	3824.0
178.00	167.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

m/z	Abundance
36.00	642.0
37.00	3952.0
38.00	3870.0
39.00	1480.0
39.90	706.0
40.90	115.0
42.90	146.0
44.00	1067.0
45.00	858.0
45.90	235.0
47.00	798.0
47.80	468.0
49.00	3613.0
50.00	16266.0
51.00	5045.0
51.90	196.0
55.00	320.0
56.00	1783.0
57.00	3062.0
57.90	167.0
60.00	808.0
61.10	4542.0
62.00	4390.0
63.00	3423.0
63.90	347.0
67.00	269.0
68.00	8975.0
69.00	9895.0
70.00	760.0
72.10	495.0
73.00	4759.0
74.00	17296.0
75.00	48792.0
76.00	4034.0
77.10	495.0
77.90	421.0
78.90	4435.0
79.90	1064.0
80.90	4550.0
81.90	828.0
82.80	166.0
87.00	3664.0
88.00	3432.0
91.00	430.0
92.00	3026.0
93.00	4315.0
94.00	11833.0
95.00	89072.0
96.00	5920.0
97.00	210.0
103.90	501.0
104.90	149.0
105.80	557.0
106.80	137.0
109.80	125.0
110.80	160.0
112.90	111.0
115.80	345.0
116.90	857.0
117.90	503.0
118.80	461.0
123.90	100.0
127.90	433.0
128.80	154.0
129.80	343.0
131.00	165.0
134.80	190.0
136.90	237.0
139.90	124.0
140.90	1251.0
142.90	1181.0
145.20	105.0
145.70	137.0
147.90	245.0
154.80	259.0
156.80	127.0
158.80	149.0
171.50	175.0
172.10	266.0
174.00	67496.0
175.00	5167.0
176.00	65640.0
176.90	3915.0
178.00	176.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

m/z	Abundance
40.00	633.0
41.00	108.0
44.00	251.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69