

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022820\
 Data File : VV014718.D
 Acq On : 28 Feb 2020 19:42
 Operator : SY/MD
 Sample : L1730-02
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0XT8

Quant Time: Feb 28 23:54:45 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Feb 28 23:36:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	270286	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	259040	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	126334	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	102056	4.82	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.40%
7) Chloroethane-d5	1.58	69	83114	5.02	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.40%
11) 1,1-Dichloroethene-d2	2.13	63	131071	3.64	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.80%
20) 2-Butanone-d5	3.97	46	211109	48.27	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.54%
24) Chloroform-d	4.40	84	181901	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.80%
26) 1,2-Dichloroethane-d4	5.08	65	97293	5.22	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.40%
32) Benzene-d6	5.09	84	374414	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.80%
36) 1,2-Dichloropropane-d6	6.11	67	117352	4.99	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.80%
41) Toluene-d8	7.35	98	334991	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
43) trans-1,3-Dichloropropene-	7.66	79	41932	4.62	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.40%
46) 2-Hexanone-d5	8.13	63	176844	48.10	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.20%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	80932	4.81	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	116916	4.98	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.60%


Target Compounds					Ovalue
3) Chloromethane	1.25	50	5040	0.184 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV022820\
Data File : VV014718.D
Acq On : 28 Feb 2020 19:42
Operator : SY/MD
Sample : L1730-02
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0XT8

Quant Time: Feb 28 23:54:45 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Feb 28 23:36:40 2020
Response via : Initial Calibration

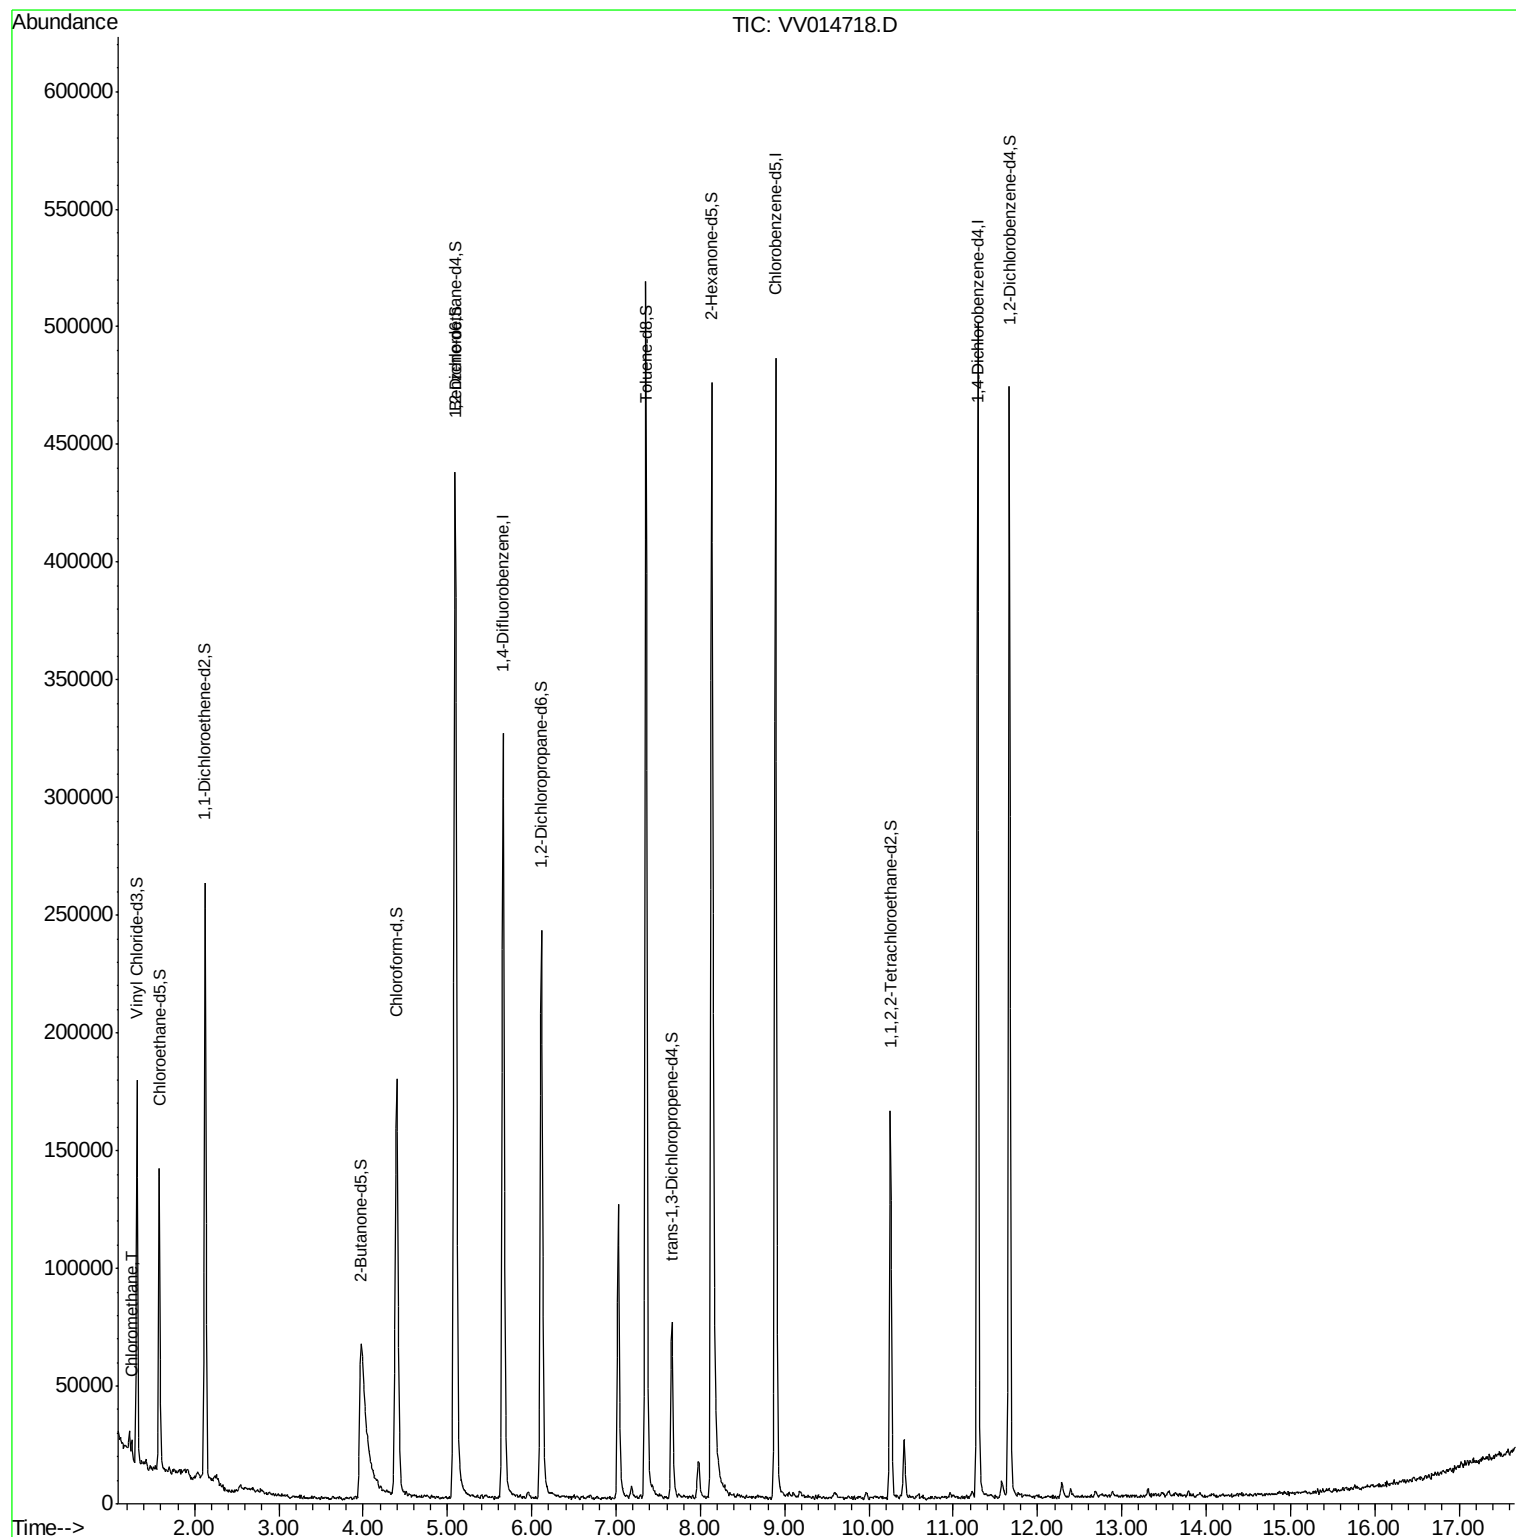

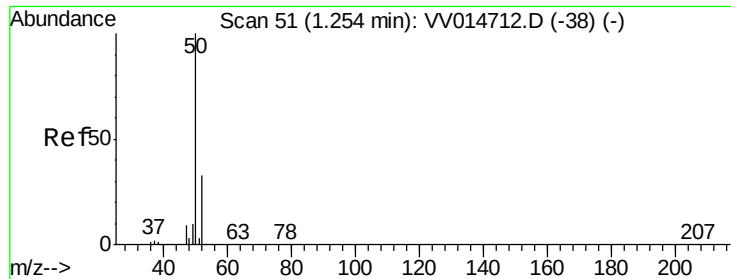

#3
 Chloromethane
 Concen: 0.184 ug/L
 RT: 1.25 min Scan# 50
 Delta R.T. -0.00 min
 Lab File: VV014718.D
 Acq: 28 Feb 2020 19:42

Instrument :
 MSVOA_V
 ClientSampleId :
 C0XT8

Tot Ion: 50 Resp: 5040
 Ion Ratio Lower Upper
 50 100
 52 32.7 22.9 42.5

