

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022820\
 Data File : VV014719.D
 Acq On : 28 Feb 2020 20:06
 Operator : SY/MD
 Sample : L1730-03
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0XT9

Quant Time: Feb 28 23:57:21 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Feb 28 23:36:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	259056	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	247057	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	118603	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	98706	4.87	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.40%
7) Chloroethane-d5	1.58	69	78515	4.95	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.00%
11) 1,1-Dichloroethene-d2	2.13	63	124572	3.61	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.20%
20) 2-Butanone-d5	3.98	46	187785	44.79	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.58%
24) Chloroform-d	4.40	84	175624	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.40%
26) 1,2-Dichloroethane-d4	5.08	65	93559	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.80%
32) Benzene-d6	5.10	84	362567	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.20%
36) 1,2-Dichloropropane-d6	6.11	67	113237	5.05	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.00%
41) Toluene-d8	7.35	98	321323	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.00%
43) trans-1,3-Dichloropropene-	7.66	79	42399	4.89	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.80%
46) 2-Hexanone-d5	8.14	63	172635	49.23	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.46%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	79534	4.96	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	114507	5.20	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.00%


Target Compounds					Ovalue
3) Chloromethane	1.25	50	4763	0.182 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV022820\
Data File : VV014719.D
Acq On : 28 Feb 2020 20:06
Operator : SY/MD
Sample : L1730-03
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0XT9

Quant Time: Feb 28 23:57:21 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Feb 28 23:36:40 2020
Response via : Initial Calibration

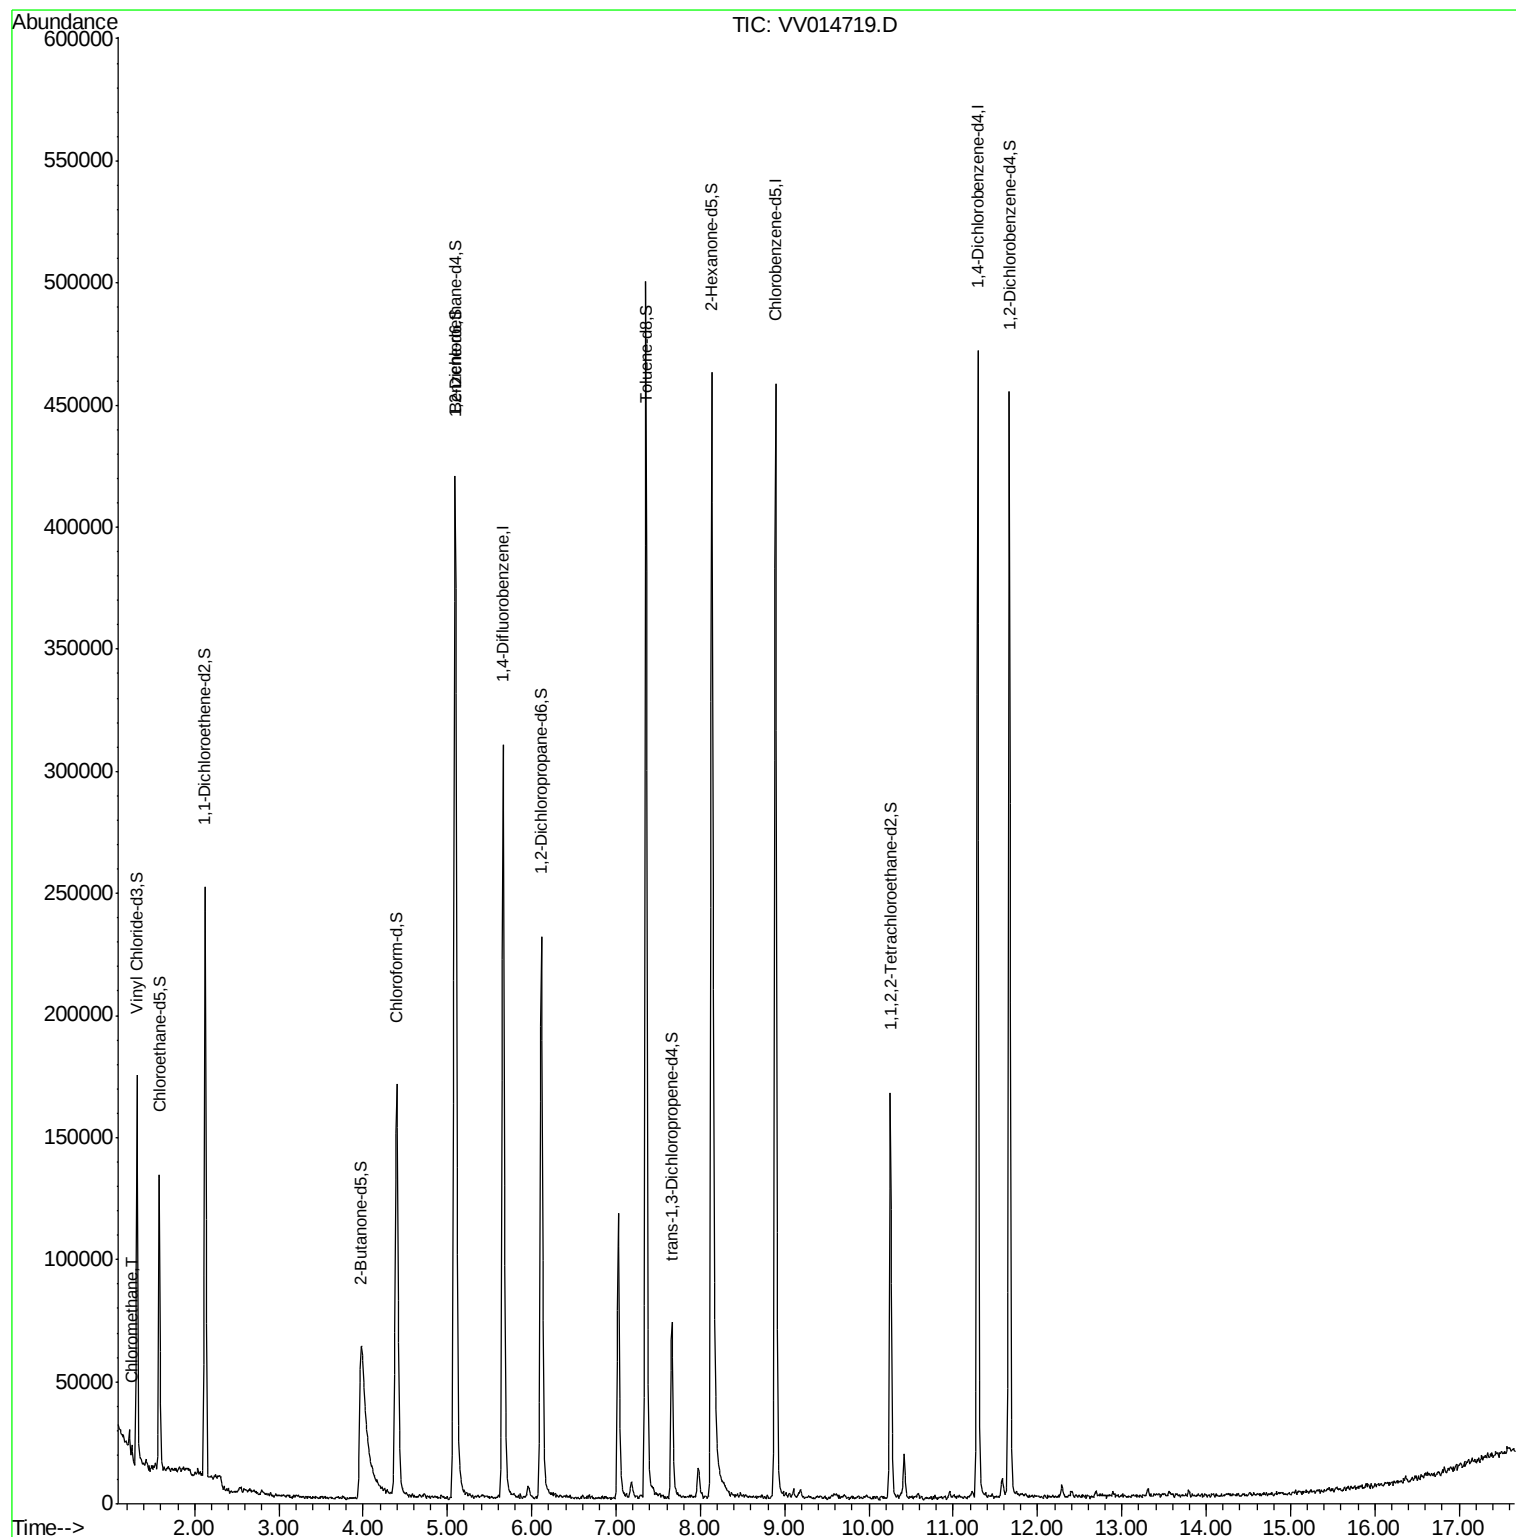

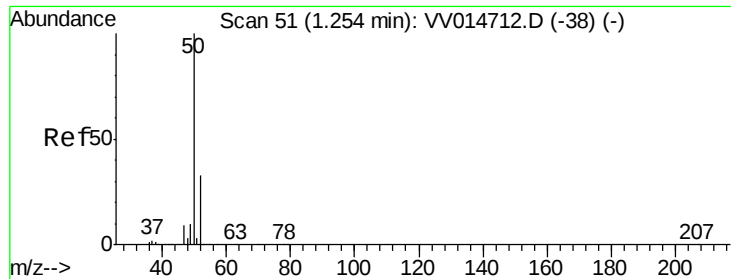

#3
 Chloromethane
 Concen: 0.182 ug/L
 RT: 1.25 min Scan# 50
 Delta R.T. -0.00 min
 Lab File: VV014719.D
 Acq: 28 Feb 2020 20:06

Instrument :
 MSVOA_V
 ClientSampleId :
 C0XT9

Tot Ion: 50 Resp: 4763
 Ion Ratio Lower Upper
 50 100
 52 39.0 22.9 42.5

