

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV022820\
 Data File : VV014721.D
 Acq On : 28 Feb 2020 20:53
 Operator : SY/MD
 Sample : L1730-06
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0XW2

Quant Time: Feb 29 00:05:14 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Feb 28 23:36:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	258419	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	247603	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	120470	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	97550	4.82	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.40%
7) Chloroethane-d5	1.58	69	78222	4.94	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.80%
11) 1,1-Dichloroethene-d2	2.13	63	126172	3.67	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.40%
20) 2-Butanone-d5	3.98	46	204148	48.82	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.64%
24) Chloroform-d	4.40	84	177030	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.60%
26) 1,2-Dichloroethane-d4	5.08	65	93938	5.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.60%
32) Benzene-d6	5.09	84	364439	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.60%
36) 1,2-Dichloropropane-d6	6.11	67	115448	5.14	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.80%
41) Toluene-d8	7.35	98	324679	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.80%
43) trans-1,3-Dichloropropene-	7.66	79	40746	4.69	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.80%
46) 2-Hexanone-d5	8.14	63	167245	47.59	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.18%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	79337	4.94	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	116243	5.20	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.00%


Target Compounds					Ovalue
3) Chloromethane	1.25	50	3243	0.124 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV022820\
Data File : VV014721.D
Acq On : 28 Feb 2020 20:53
Operator : SY/MD
Sample : L1730-06
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0XW2

Quant Time: Feb 29 00:05:14 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Feb 28 23:36:40 2020
Response via : Initial Calibration

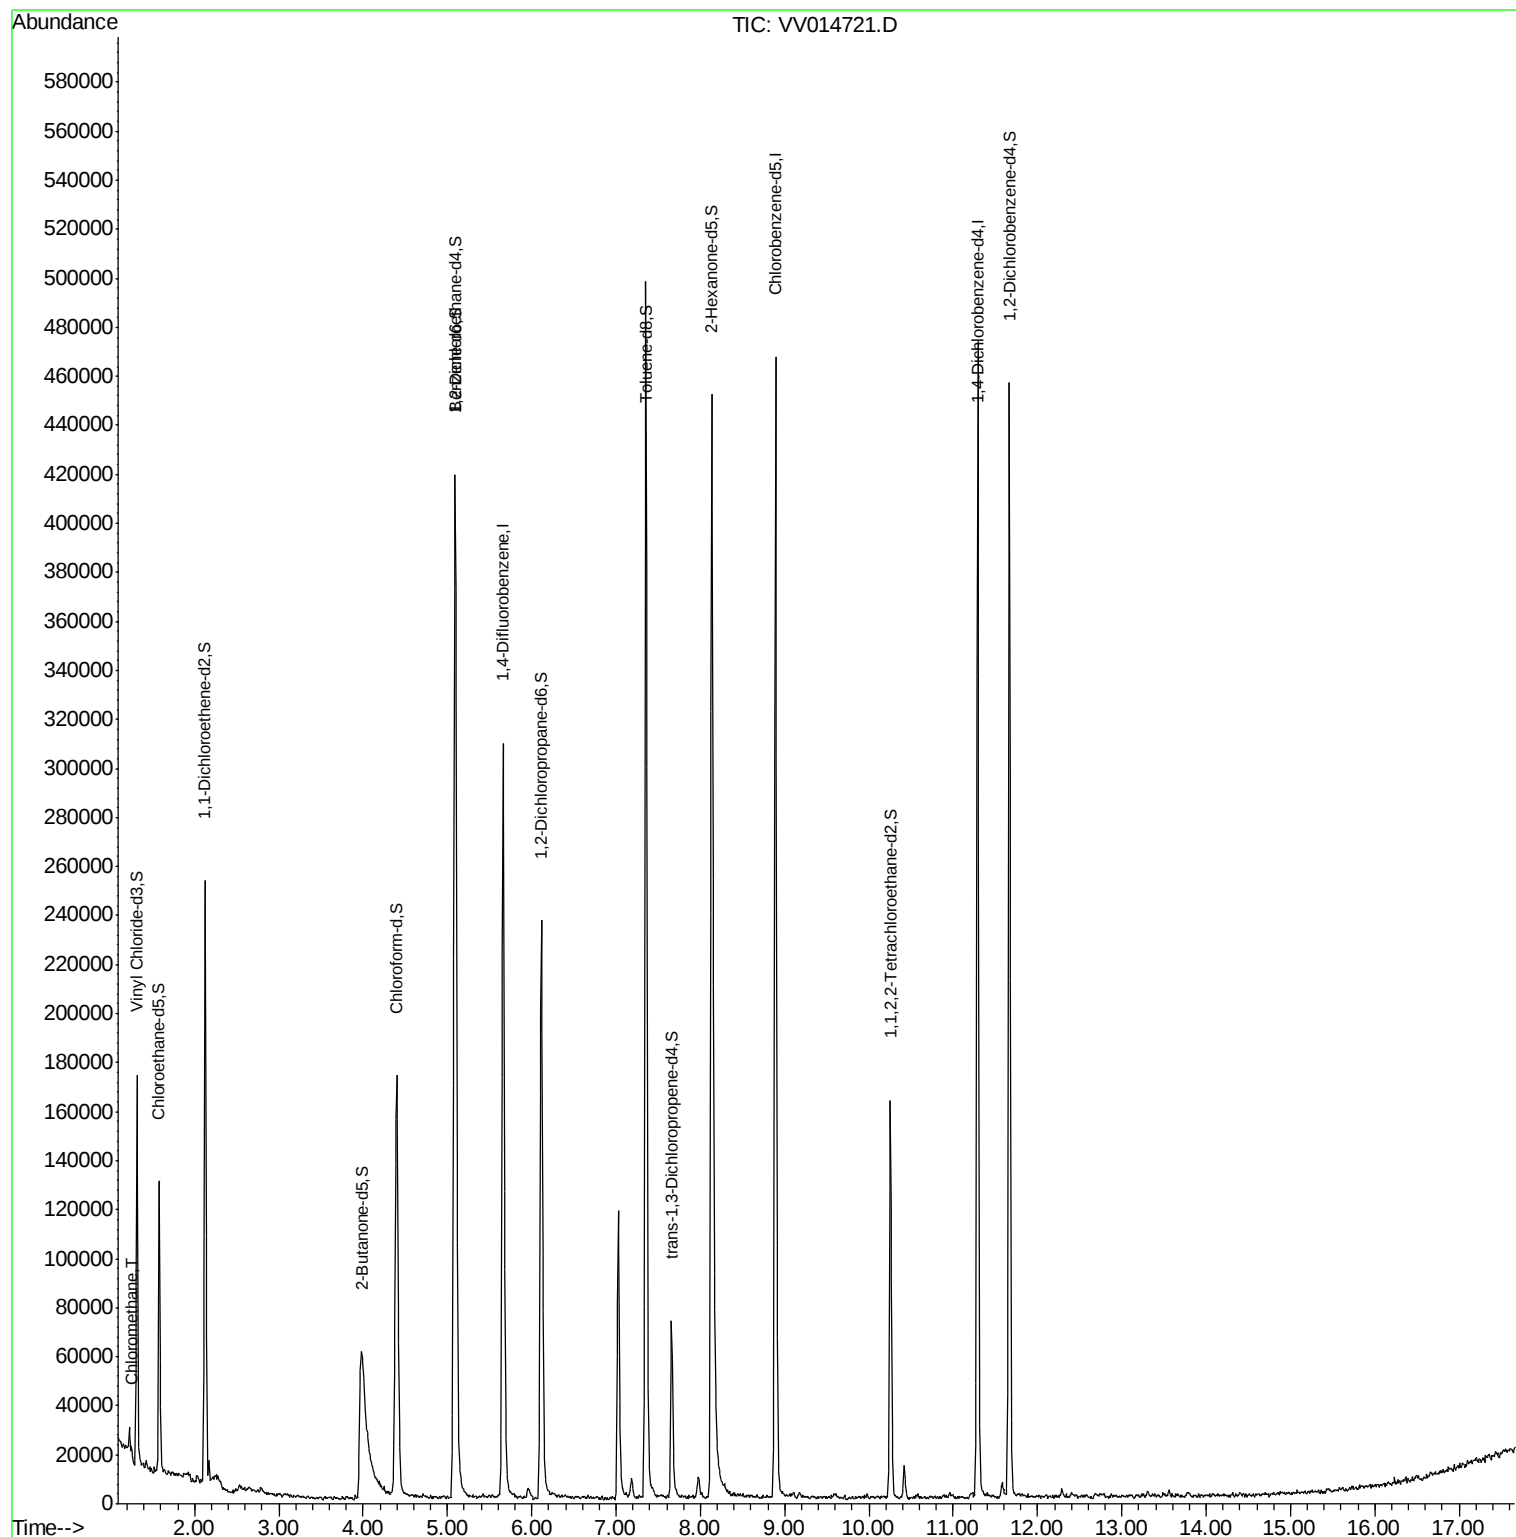

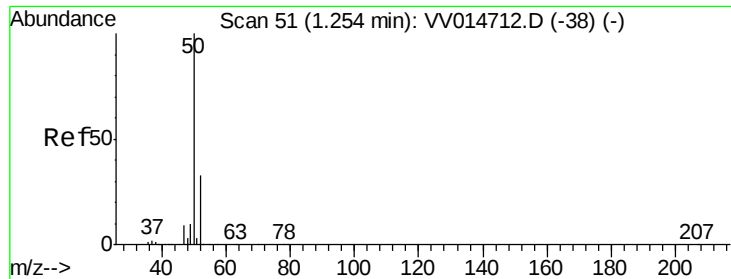

#3
 Chloromethane
 Concen: 0.124 ug/L
 RT: 1.25 min Scan# 51
 Delta R.T. 0.00 min
 Lab File: VV014721.D
 Acq: 28 Feb 2020 20:53

Instrument :
 MSVOA_V
 ClientSampleId :
 C0XW2

Tot Ion: 50 Resp: 3243
 Ion Ratio Lower Upper
 50 100
 52 37.9 22.9 42.5

