


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV022820\
 Data File : VV014709.D
 Acq On : 28 Feb 2020 15:17
 Operator : SY/MD
 Sample : BFB39
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB39

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022820WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Feb 28 23:36:40 2020

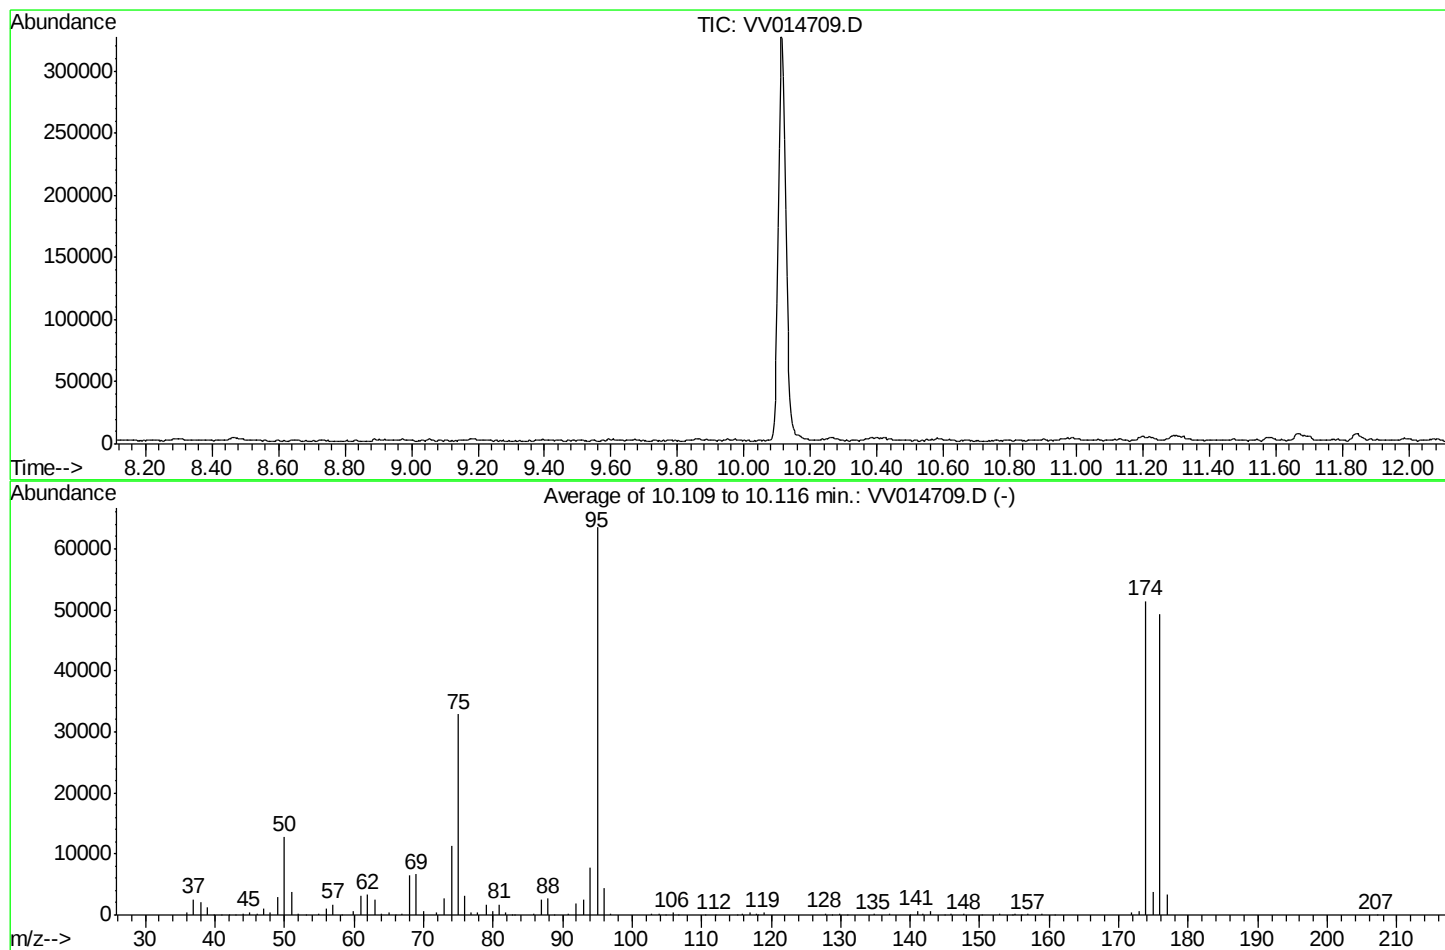

AutoFind: Scans 2805, 2806, 2807; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	12898	PASS
75	95	30	80	51.8	32885	PASS
95	95	100	100	100.0	63496	PASS
96	95	5	9	6.9	4351	PASS
173	174	0.00	2	1.4	737	PASS
174	95	50	120	81.1	51464	PASS
175	174	5	9	7.2	3690	PASS
176	174	95	101	95.6	49184	PASS
177	176	5	9	6.6	3266	PASS

m/z	Abundance
35.90	623.0
37.00	2670.0
38.00	2312.0
39.00	1347.0
39.90	613.0
41.00	143.0
42.00	124.0
42.90	154.0
44.00	991.0
44.90	445.0
46.10	156.0
47.00	1058.0
47.90	353.0
49.00	2895.0
50.00	12202.0
51.00	3632.0
52.10	201.0
54.90	330.0
56.00	925.0
57.00	1542.0
59.90	669.0
61.00	2936.0
62.00	2966.0
63.00	2288.0
64.00	323.0
65.10	320.0
66.90	269.0
68.00	6008.0
69.00	6270.0
70.00	588.0
72.00	390.0
73.00	2766.0
74.00	10668.0
75.00	30856.0
76.00	2815.0
76.90	574.0
77.70	390.0
79.00	1758.0
79.90	618.0
81.00	1666.0
81.80	371.0
83.10	107.0
85.80	125.0
86.90	2336.0
88.00	2454.0
88.80	105.0
90.80	253.0
91.90	1555.0
93.00	2370.0
94.00	7423.0
95.00	59728.0
96.00	4284.0
96.90	198.0
102.70	120.0
103.90	270.0
104.80	114.0
105.80	322.0
115.10	104.0
115.90	218.0
116.90	371.0
118.10	187.0
119.00	362.0
127.80	274.0
128.80	146.0
129.80	267.0
134.90	111.0
137.00	113.0
141.00	724.0
141.90	139.0
143.00	613.0
145.00	127.0
145.90	154.0
147.80	231.0
152.90	151.0
154.70	139.0
155.00	153.0
155.90	121.0
157.00	145.0
158.90	203.0
160.80	128.0
171.80	496.0
173.00	712.0
173.90	47744.0
174.90	3504.0
175.90	44472.0
176.90	2778.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39

m/z	Abundance
35.90	664.0
37.00	2769.0
38.00	2371.0
39.00	1440.0
39.90	608.0
40.90	176.0
42.10	128.0
42.90	176.0
44.00	1071.0
44.90	524.0
46.10	153.0
47.00	1128.0
48.00	420.0
49.00	3195.0
50.00	13374.0
51.00	4011.0
52.00	243.0
53.00	112.0
54.90	366.0
56.00	1026.0
57.00	1747.0
58.20	119.0
59.90	692.0
61.00	3231.0
62.00	3358.0
63.00	2714.0
63.90	290.0
65.10	372.0
66.00	110.0
66.90	275.0
68.00	6782.0
69.00	6990.0
70.00	642.0
71.90	386.0
73.00	2999.0
74.00	11805.0
75.00	34064.0
76.00	3264.0
76.90	554.0
77.80	342.0
78.90	1851.0
79.90	700.0
81.00	1850.0
81.80	422.0
83.10	110.0
85.80	158.0
86.90	2562.0
88.00	2766.0
90.80	292.0
91.90	1975.0
93.00	2588.0
94.00	7896.0
95.00	66080.0
96.00	4514.0
96.90	166.0
102.70	131.0
103.90	291.0
105.90	358.0
106.70	112.0
115.10	125.0
115.90	303.0
117.00	395.0
117.80	235.0
119.00	415.0
127.80	305.0
128.70	121.0
129.90	257.0
130.90	121.0
134.80	129.0
137.00	120.0
140.00	104.0
141.00	749.0
141.90	148.0
143.00	669.0
145.00	102.0
145.90	177.0
147.70	202.0
150.20	110.0
152.80	155.0
155.00	188.0
155.90	126.0
157.00	199.0
158.80	145.0
160.80	104.0
171.80	472.0
173.00	775.0
173.90	53136.0
174.90	3843.0
175.90	50656.0
176.90	3309.0
207.10	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39

m/z	Abundance
36.00	611.0
37.00	2643.0
38.00	2200.0
39.00	1306.0
39.90	638.0
40.90	170.0
42.10	118.0
42.90	216.0
44.00	1165.0
44.90	509.0
46.10	154.0
47.10	1109.0
47.90	460.0
49.00	3009.0
50.00	13118.0
51.00	3980.0
52.00	259.0
53.00	127.0
54.90	368.0
55.90	1015.0
57.00	1851.0
58.10	123.0
59.90	684.0
61.00	3138.0
62.00	3530.0
63.00	2762.0
64.00	281.0
65.10	402.0
66.00	128.0
66.90	251.0
68.00	6903.0
69.00	6824.0
70.00	558.0
71.90	358.0
73.00	2944.0
74.00	11705.0
75.00	33736.0
76.00	3396.0
76.90	465.0
77.90	293.0
78.90	1729.0
79.90	732.0
80.90	1834.0
81.80	405.0
82.80	105.0
85.80	211.0
86.90	2516.0
87.90	2838.0
90.70	298.0
91.90	2122.0
93.00	2678.0
94.00	7676.0
95.00	64680.0
96.00	4256.0
96.90	106.0
102.70	131.0
103.90	275.0
105.90	380.0
106.70	149.0
110.60	110.0
111.90	127.0
115.00	105.0
115.80	351.0
117.00	378.0
117.80	314.0
118.90	422.0
127.80	263.0
129.90	234.0
130.90	168.0
134.70	139.0
136.90	123.0
141.00	713.0
141.90	147.0
143.00	683.0
144.90	106.0
146.00	166.0
147.70	168.0
150.20	111.0
152.80	129.0
155.00	209.0
156.90	225.0
158.90	115.0
171.80	415.0
173.00	725.0
173.90	53512.0
174.90	3724.0
175.90	52424.0
176.90	3711.0
207.10	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39

m/z	Abundance
35.10	162.0
35.90	156.0
36.80	107.0
37.90	112.0
39.10	164.0
40.00	518.0
40.90	114.0
41.60	158.0
42.20	105.0
43.00	141.0
44.00	787.0
45.70	102.0
55.10	145.0
72.90	134.0
102.20	107.0
124.80	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39