

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022823\
 Data File : VW030093.D
 Acq On : 28 Feb 2023 12:41
 Operator : SY/MD
 Sample : 01729-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BZ7

Quant Time: Mar 01 00:05:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 01 00:04:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	229173	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	212303	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	114195	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	63228	4.264	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.200%
7) Chloroethane-d5	1.539	69	62831	4.514	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.200%
11) 1,1-Dichloroethene-d2	2.066	63	98744	3.239	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.800%
20) 2-Butanone-d5	3.815	46	120786	44.180	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.360%
24) Chloroform-d	4.256	84	130025	4.293	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.800%
26) 1,2-Dichloroethane-d4	4.950	65	56886	4.600	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.000%
32) Benzene-d6	4.966	84	260891	4.567	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.400%
36) 1,2-Dichloropropane-d6	5.995	67	79686	4.637	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.800%
41) Toluene-d8	7.249	98	236693	4.371	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.400%
43) trans-1,3-Dichloroprop...	7.558	79	27140	4.616	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.400%
46) 2-Hexanone-d5	8.030	63	112129	46.095	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.200%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	55419	4.533	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.600%
66) 1,2-Dichlorobenzene-d4	11.570	152	92515	4.788	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.800%
Target Compounds						Qvalue
16) Methylene chloride	2.455	84	4759	0.253	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022823\
Data File : VV030093.D
Acq On : 28 Feb 2023 12:41
Operator : SY/MD
Sample : 01729-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COBZ7

Quant Time: Mar 01 00:05:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 01 00:04:57 2023
Response via : Initial Calibration

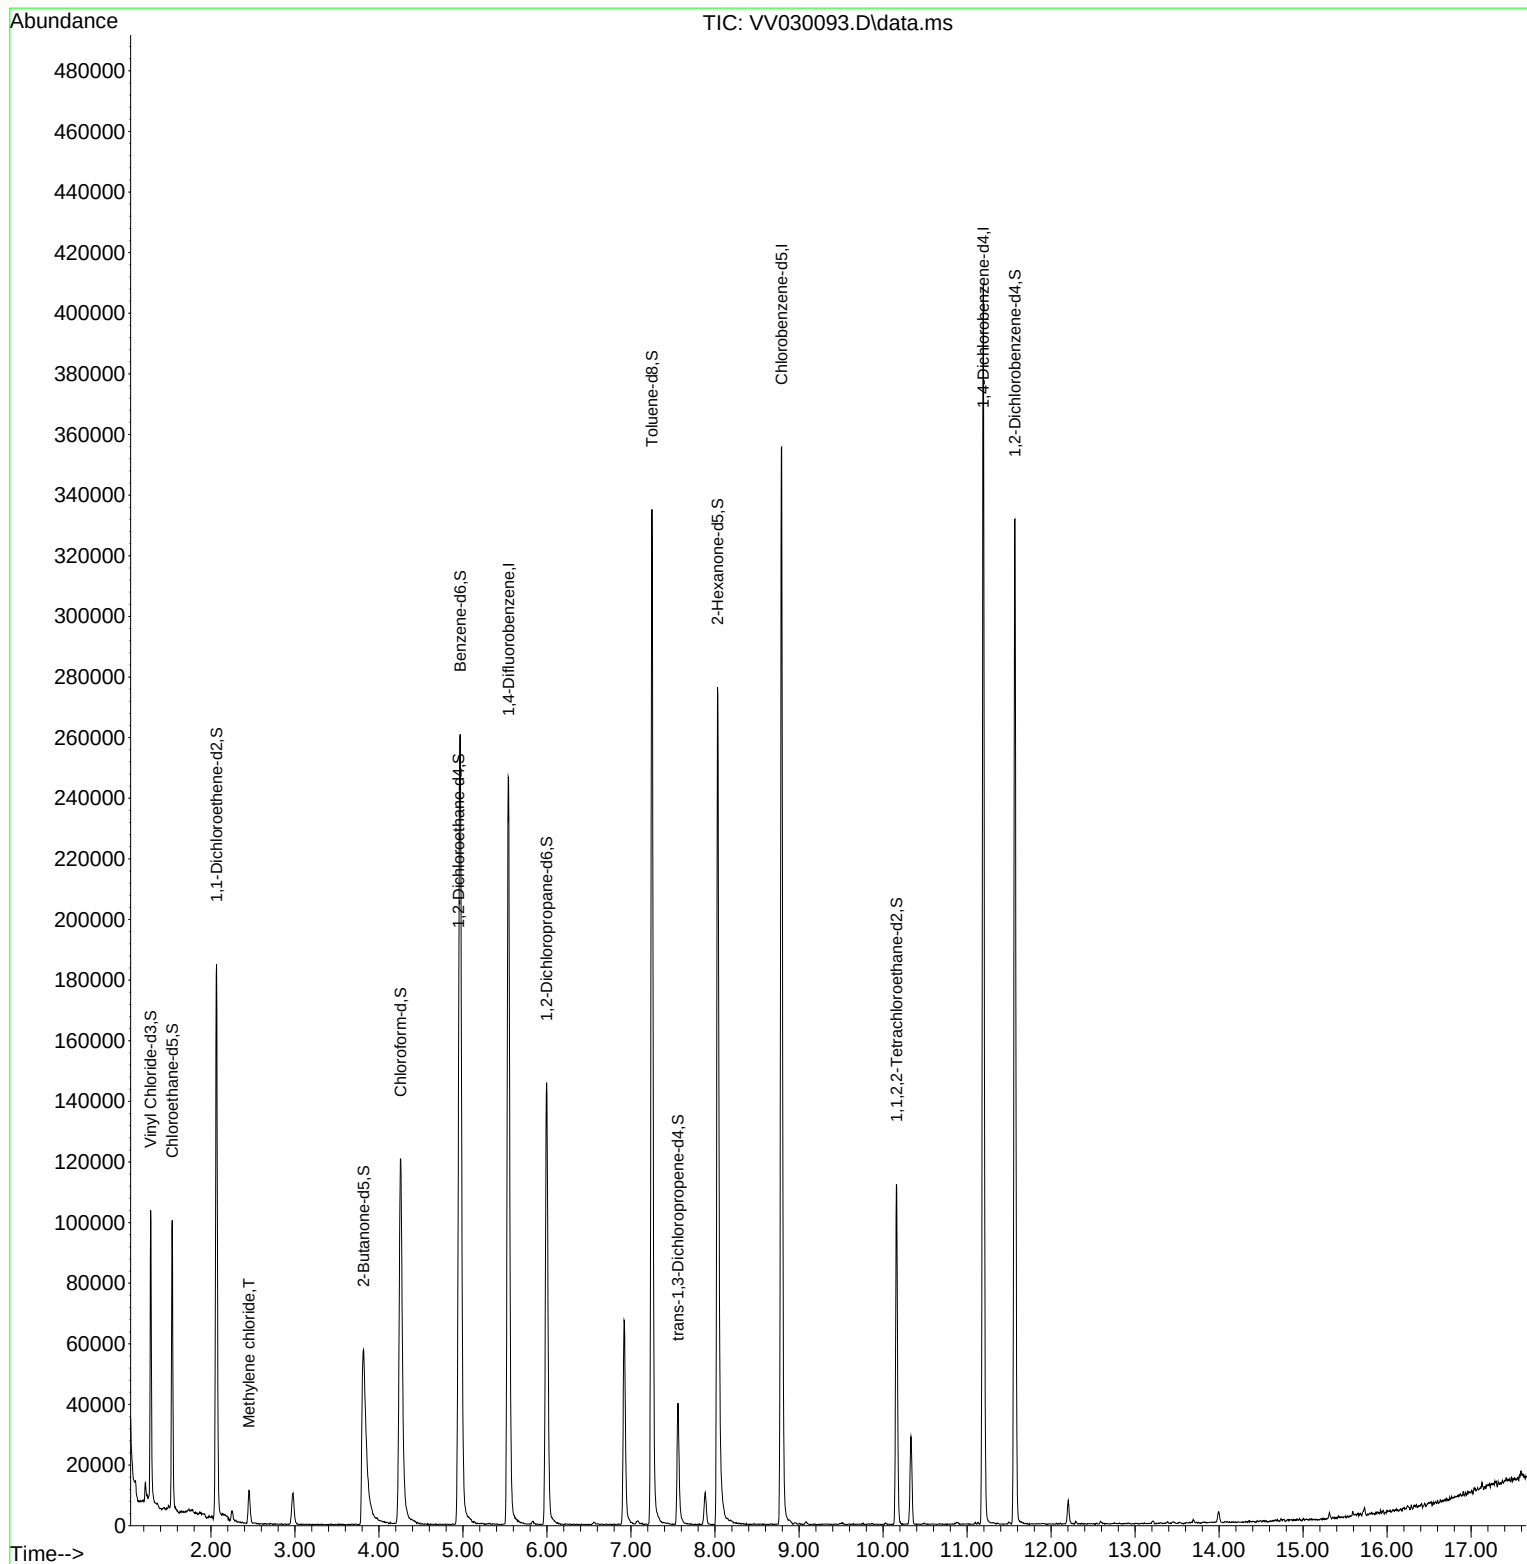

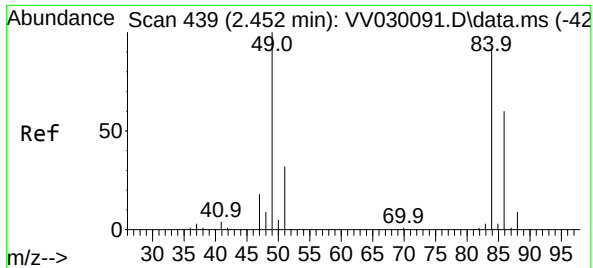

#16
Methylene chloride
Concen: 0.253 ug/L
RT: 2.455 min Scan# 44
Delta R.T. 0.003 min
Lab File: VV030093.D
Acq: 28 Feb 2023 12:41

Instrument :
MSVOA_V
ClientSampleId :
C0BZ7

Tgt Ion:	84	Resp:	4759
Ion	Ratio	Lower	Upper
84	100		
86	72.1	44.7	83.1
49	110.8	78.8	146.3

