

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022823\
 Data File : VW030096.D
 Acq On : 28 Feb 2023 13:52
 Operator : SY/MD
 Sample : 01729-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BY6

Quant Time: Mar 01 00:06:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 01 00:04:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	181077	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	172719	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	90578	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	54734	4.671	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.400%
7) Chloroethane-d5	1.539	69	54336	4.940	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.800%
11) 1,1-Dichloroethene-d2	2.066	63	85411	3.546	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.000%
20) 2-Butanone-d5	3.822	46	109916	50.883	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.760%
24) Chloroform-d	4.262	84	117761	4.920	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.400%
26) 1,2-Dichloroethane-d4	4.957	65	51634	5.285	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.600%
32) Benzene-d6	4.973	84	230605	4.962	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.200%
36) 1,2-Dichloropropane-d6	5.998	67	71287	5.099	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.000%
41) Toluene-d8	7.252	98	206510	4.688	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.800%
43) trans-1,3-Dichloroprop...	7.561	79	24009	5.019	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	100.400%
46) 2-Hexanone-d5	8.034	63	106185	53.656	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.320%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	51670	5.195	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.800%
66) 1,2-Dichlorobenzene-d4	11.570	152	82370	5.375	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.400%
Target Compounds						
					Qvalue	
25) Chloroform	4.288	83	18628	0.832	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022823\
Data File : VV030096.D
Acq On : 28 Feb 2023 13:52
Operator : SY/MD
Sample : 01729-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BY6

Quant Time: Mar 01 00:06:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 01 00:04:57 2023
Response via : Initial Calibration

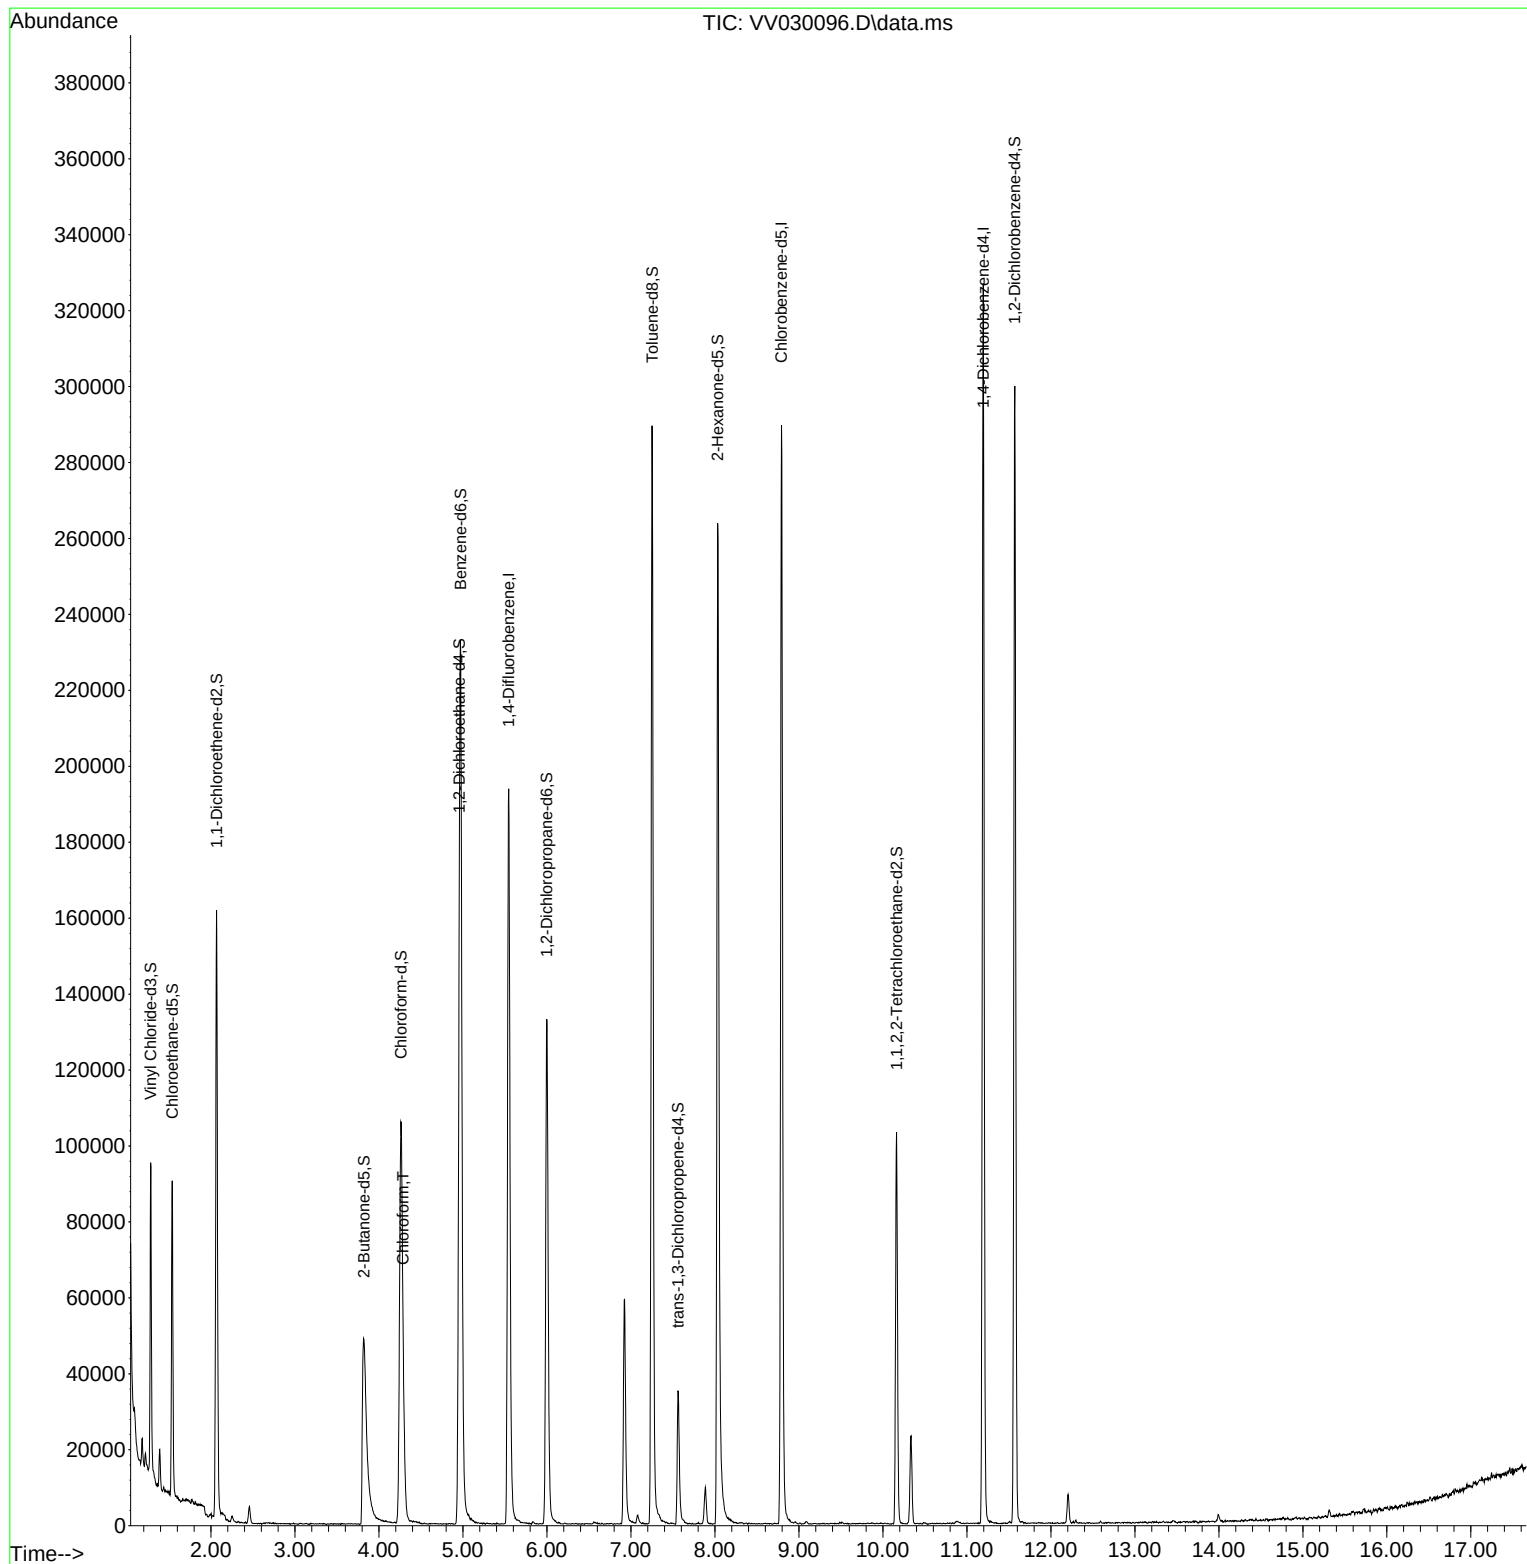

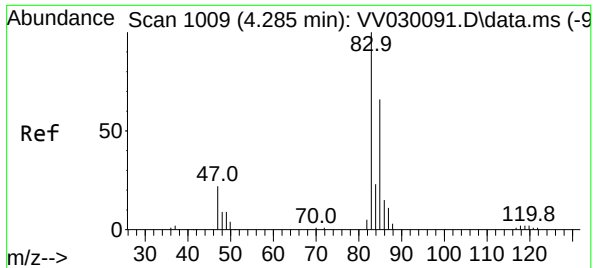

#25

Chloroform

Concen: 0.832 ug/L

RT: 4.288 min Scan# 10

Delta R.T. 0.003 min

Lab File: VV030096.D

Acq: 28 Feb 2023 13:52

Instrument :

MSVOA_V

ClientSampleId :

C0BY6

Tgt Ion: 83 Resp: 18628

Ion Ratio Lower Upper

83 100

85 71.9 46.5 86.5

