

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022823\
 Data File : VW030097.D
 Acq On : 28 Feb 2023 14:17
 Operator : SY/MD
 Sample : 01729-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BY7

Quant Time: Mar 01 00:06:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 01 00:04:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	185993	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	177673	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	93022	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	54697	4.545	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.800%
7) Chloroethane-d5	1.539	69	53511	4.737	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.800%
11) 1,1-Dichloroethene-d2	2.066	63	86509	3.496	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.000%
20) 2-Butanone-d5	3.815	46	109928	49.543	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.080%
24) Chloroform-d	4.262	84	114513	4.658	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.200%
26) 1,2-Dichloroethane-d4	4.953	65	51824	5.164	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.200%
32) Benzene-d6	4.973	84	232991	4.873	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.400%
36) 1,2-Dichloropropane-d6	5.998	67	70077	4.872	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.400%
41) Toluene-d8	7.252	98	208053	4.591	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.800%
43) trans-1,3-Dichloroprop...	7.561	79	23906	4.858	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.200%
46) 2-Hexanone-d5	8.034	63	104438	51.302	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.600%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	50354	4.921	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.400%
66) 1,2-Dichlorobenzene-d4	11.570	152	81228	5.161	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.200%
Target Compounds						
29) 1,1,1-Trichloroethane	4.526	97	2822	0.135	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022823\
Data File : VV030097.D
Acq On : 28 Feb 2023 14:17
Operator : SY/MD
Sample : 01729-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BY7

Quant Time: Mar 01 00:06:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 01 00:04:57 2023
Response via : Initial Calibration

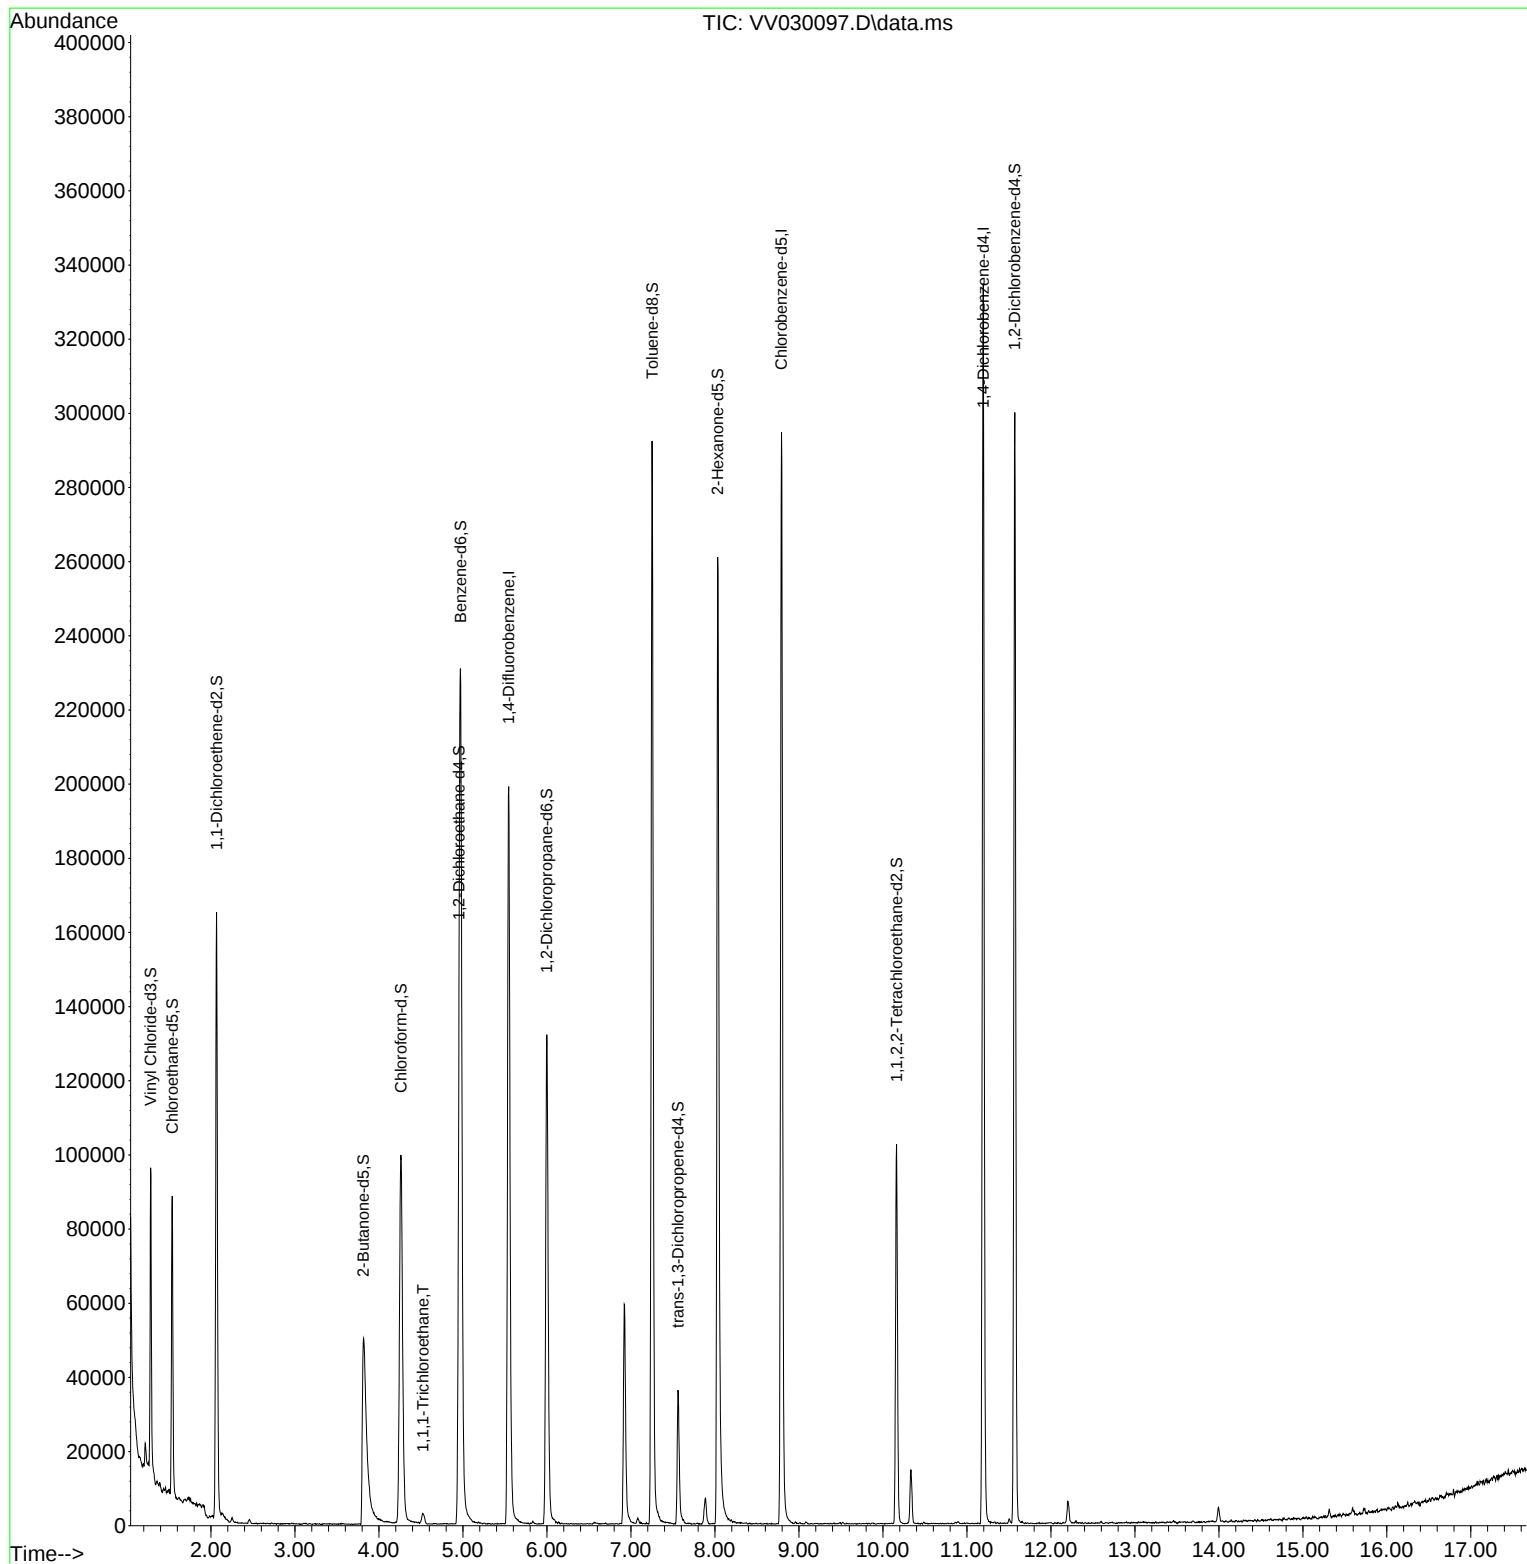

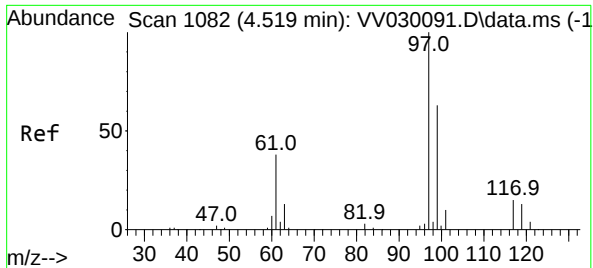

#29
 1,1,1-Trichloroethane
 Concen: 0.135 ug/L
 RT: 4.526 min Scan# 1084
 Delta R.T. 0.006 min
 Lab File: VV030097.D
 Acq: 28 Feb 2023 14:17

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BY7

Tgt Ion: 97 Resp: 2822

Ion	Ratio	Lower	Upper
97	100		
99	61.8	51.3	76.9
61	33.3	31.5	47.3

