

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022823\
 Data File : VV030094.D
 Acq On : 28 Feb 2023 13:05
 Operator : SY/MD
 Sample : 01729-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BZ5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030094.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	89	rVB	84648	95052	15.68%	1.782%
2	1.539	148	155	173	rVB	85757	103347	17.05%	1.938%
3	2.066	309	319	337	rVB	166189	243139	40.10%	4.559%
4	3.822	853	865	909	rBV2	47483	187199	30.88%	3.510%
5	4.262	983	1002	1032	rBV	103358	265704	43.83%	4.983%
6	4.969	1204	1222	1252	rBV2	236977	606266	100.00%	11.369%
7	5.545	1386	1401	1425	rBV	223642	460184	75.90%	8.630%
8	5.998	1528	1542	1570	rBV	138911	287341	47.40%	5.388%
9	6.921	1816	1829	1850	rBV	60702	114476	18.88%	2.147%
10	7.252	1919	1932	1966	rBV	300610	534454	88.16%	10.022%
11	7.561	2018	2028	2056	rBV	36365	66293	10.93%	1.243%
12	7.886	2116	2129	2139	rBV2	16741	30202	4.98%	0.566%
13	8.034	2164	2175	2217	rBV	262994	485375	80.06%	9.102%
14	8.792	2398	2411	2442	rBV	327583	545978	90.06%	10.238%
15	10.162	2826	2837	2857	rBV	103463	164920	27.20%	3.093%
16	10.336	2877	2891	2905	rVB2	33998	55807	9.21%	1.047%
17	11.194	3146	3158	3177	rBV	381455	577442	95.25%	10.828%
18	11.570	3263	3275	3294	rBV	307359	485584	80.09%	9.106%
19	12.204	3461	3472	3489	rVB2	9643	15267	2.52%	0.286%
20	13.998	4017	4030	4039	rBV	5027	8606	1.42%	0.161%




Sum of corrected areas: 5332636

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022823\
Data File : VV030094.D
Acq On : 28 Feb 2023 13:05
Operator : SY/MD
Sample : 01729-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

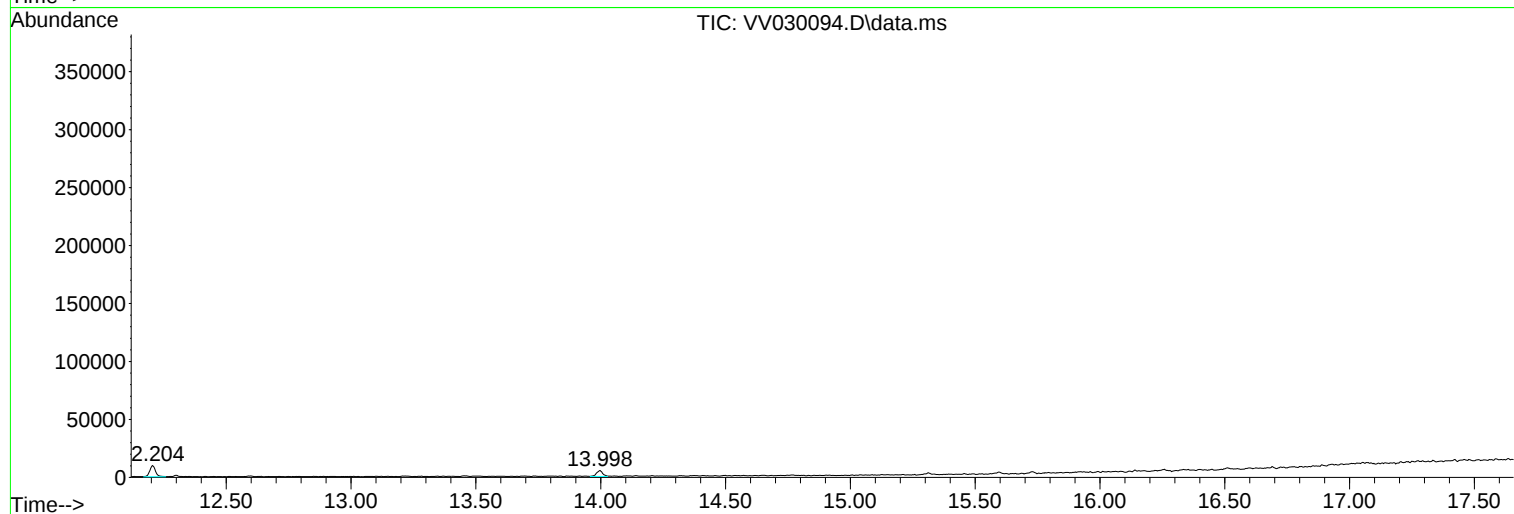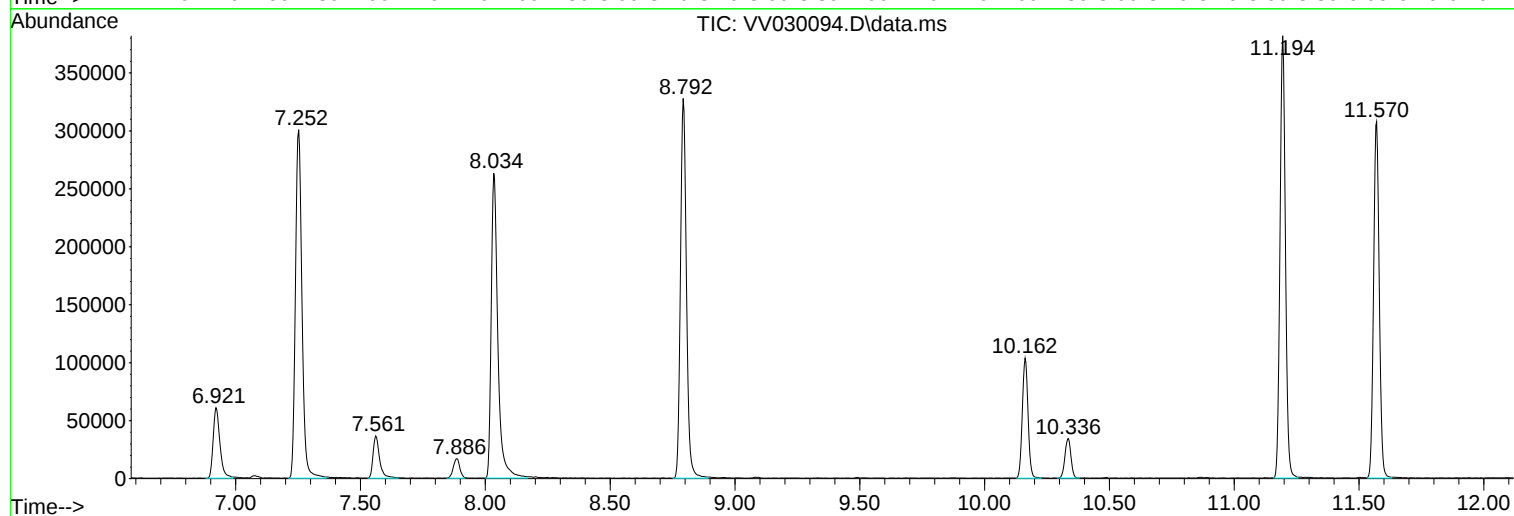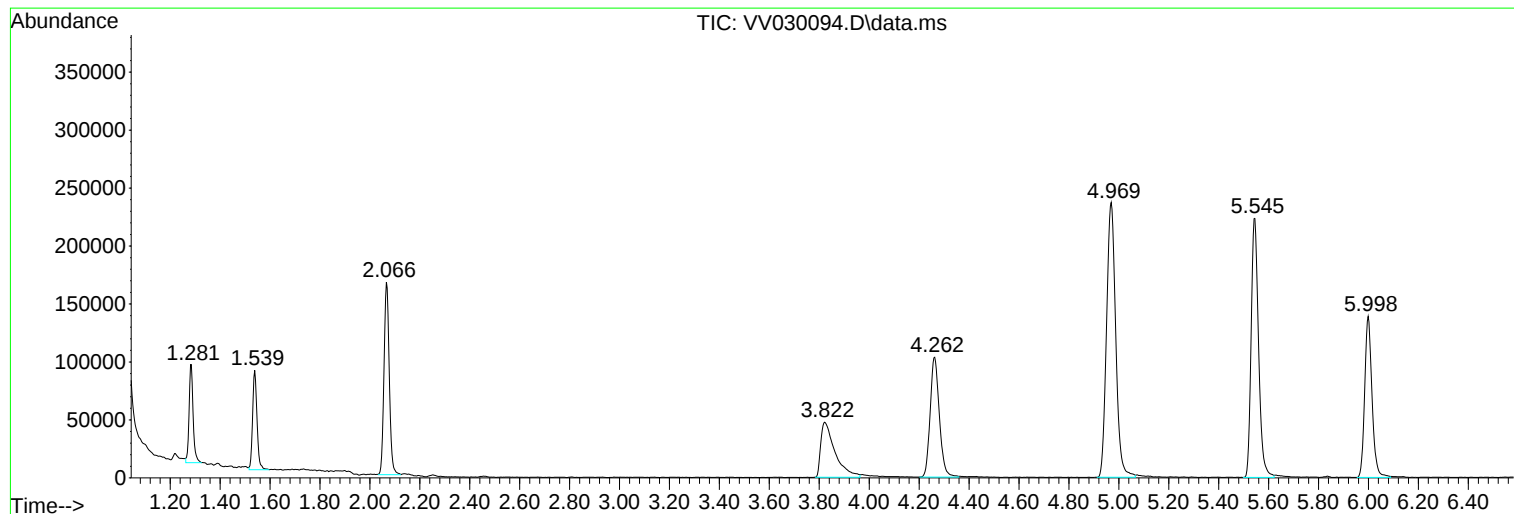

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022823\
Data File : VV030094.D
Acq On : 28 Feb 2023 13:05
Operator : SY/MD
Sample : 01729-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022823\
Data File : VV030094.D
Acq On : 28 Feb 2023 13:05
Operator : SY/MD
Sample : 01729-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc