

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022823\
 Data File : VV030097.D
 Acq On : 28 Feb 2023 14:17
 Operator : SY/MD
 Sample : 01729-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BY7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030097.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	93	rVB	85492	99613	16.73%	1.983%
2	1.539	147	155	169	rVB	81456	97502	16.38%	1.941%
3	2.066	308	319	336	rBV	163218	237746	39.94%	4.732%
4	3.818	853	864	901	rBV	50256	181340	30.46%	3.609%
5	4.262	984	1002	1026	rBV2	99144	257749	43.30%	5.130%
6	4.519	1071	1082	1100	rVB5	2921	7226	1.21%	0.144%
7	4.969	1205	1222	1269	rBV2	230628	595318	100.00%	11.849%
8	5.545	1387	1401	1429	rBV	198850	411549	69.13%	8.192%
9	5.998	1528	1542	1563	rBV	131889	273523	45.95%	5.444%
10	6.921	1818	1829	1855	rBV	59205	110537	18.57%	2.200%
11	7.252	1919	1932	1958	rBV	292109	516016	86.68%	10.271%
12	7.561	2018	2028	2046	rBV	36060	62987	10.58%	1.254%
13	7.886	2116	2129	2143	rBV	6980	13421	2.25%	0.267%
14	8.034	2163	2175	2213	rBV	260735	480742	80.75%	9.569%
15	8.792	2399	2411	2440	rBV	294395	493405	82.88%	9.821%
16	10.162	2822	2837	2856	rBV	102324	161248	27.09%	3.210%
17	10.332	2879	2890	2903	rVB2	14432	23642	3.97%	0.471%
18	11.194	3146	3158	3178	rBV	334548	520543	87.44%	10.361%
19	11.570	3263	3275	3296	rBV	299476	463346	77.83%	9.223%
20	12.201	3460	3471	3487	rBV	5867	10283	1.73%	0.205%
21	13.995	4019	4029	4039	rBV	3904	6271	1.05%	0.125%




Sum of corrected areas: 5024007

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022823\
Data File : VV030097.D
Acq On : 28 Feb 2023 14:17
Operator : SY/MD
Sample : 01729-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

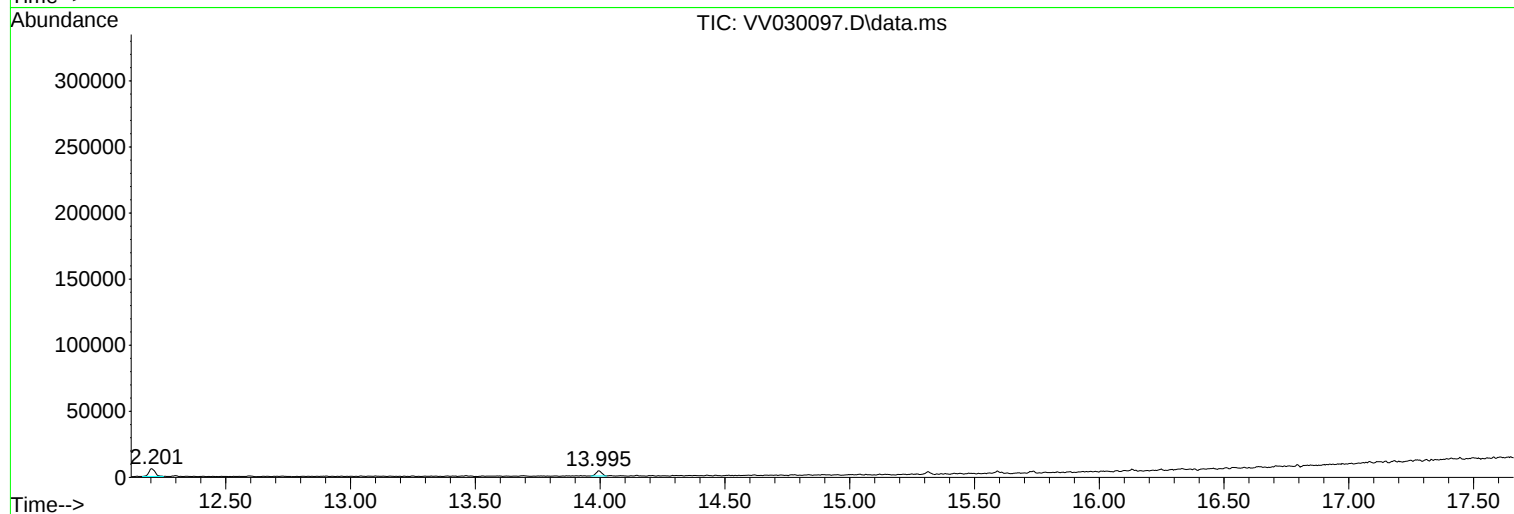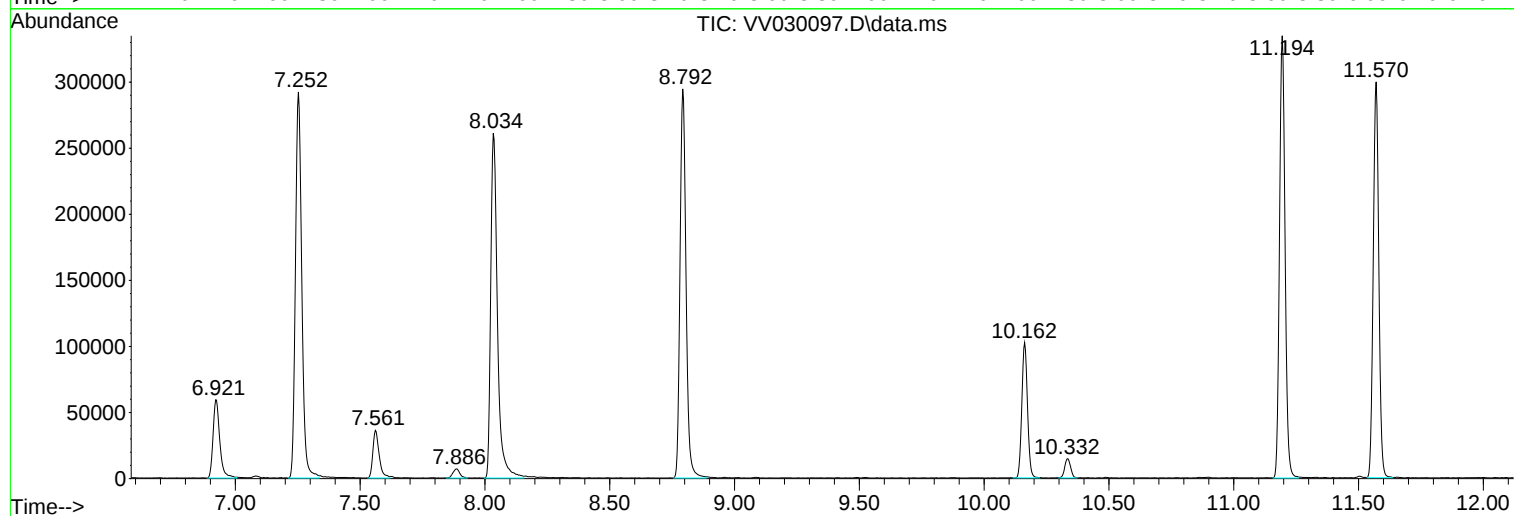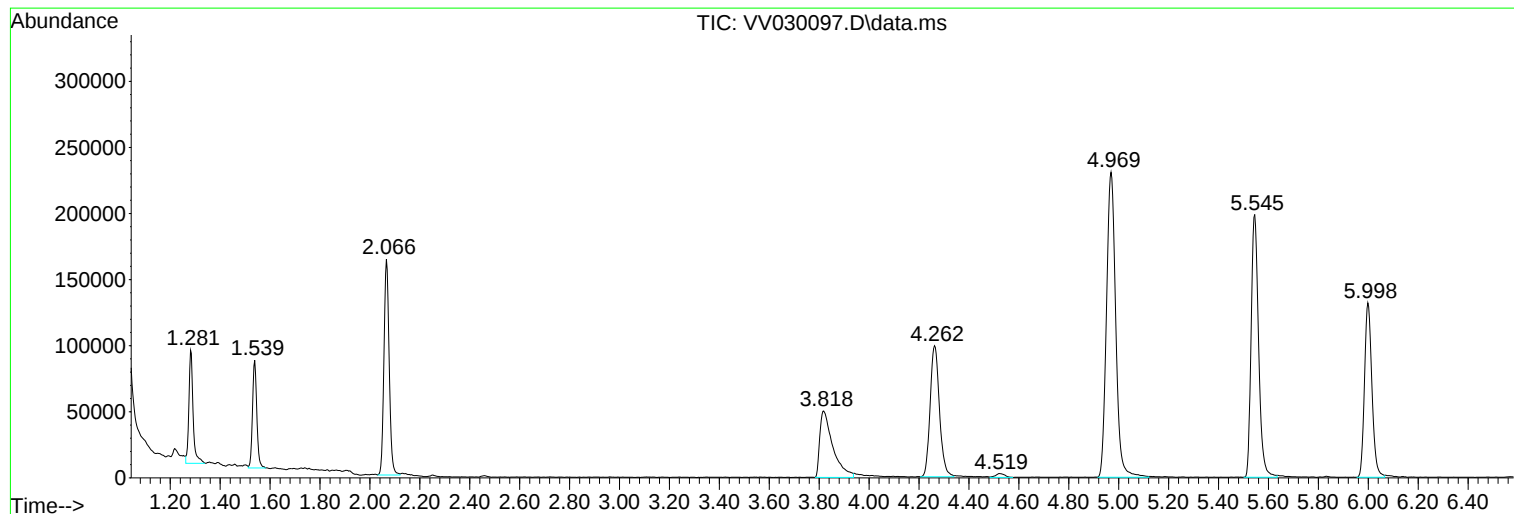

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022823\
Data File : VV030097.D
Acq On : 28 Feb 2023 14:17
Operator : SY/MD
Sample : 01729-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022823\
Data File : VV030097.D
Acq On : 28 Feb 2023 14:17
Operator : SY/MD
Sample : 01729-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
