


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022823\
Data File : VV030090.D
Acq On : 28 Feb 2023 08:56
Operator : SY/MD
Sample : BFB224
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB224

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Mar 01 00:04:57 2023

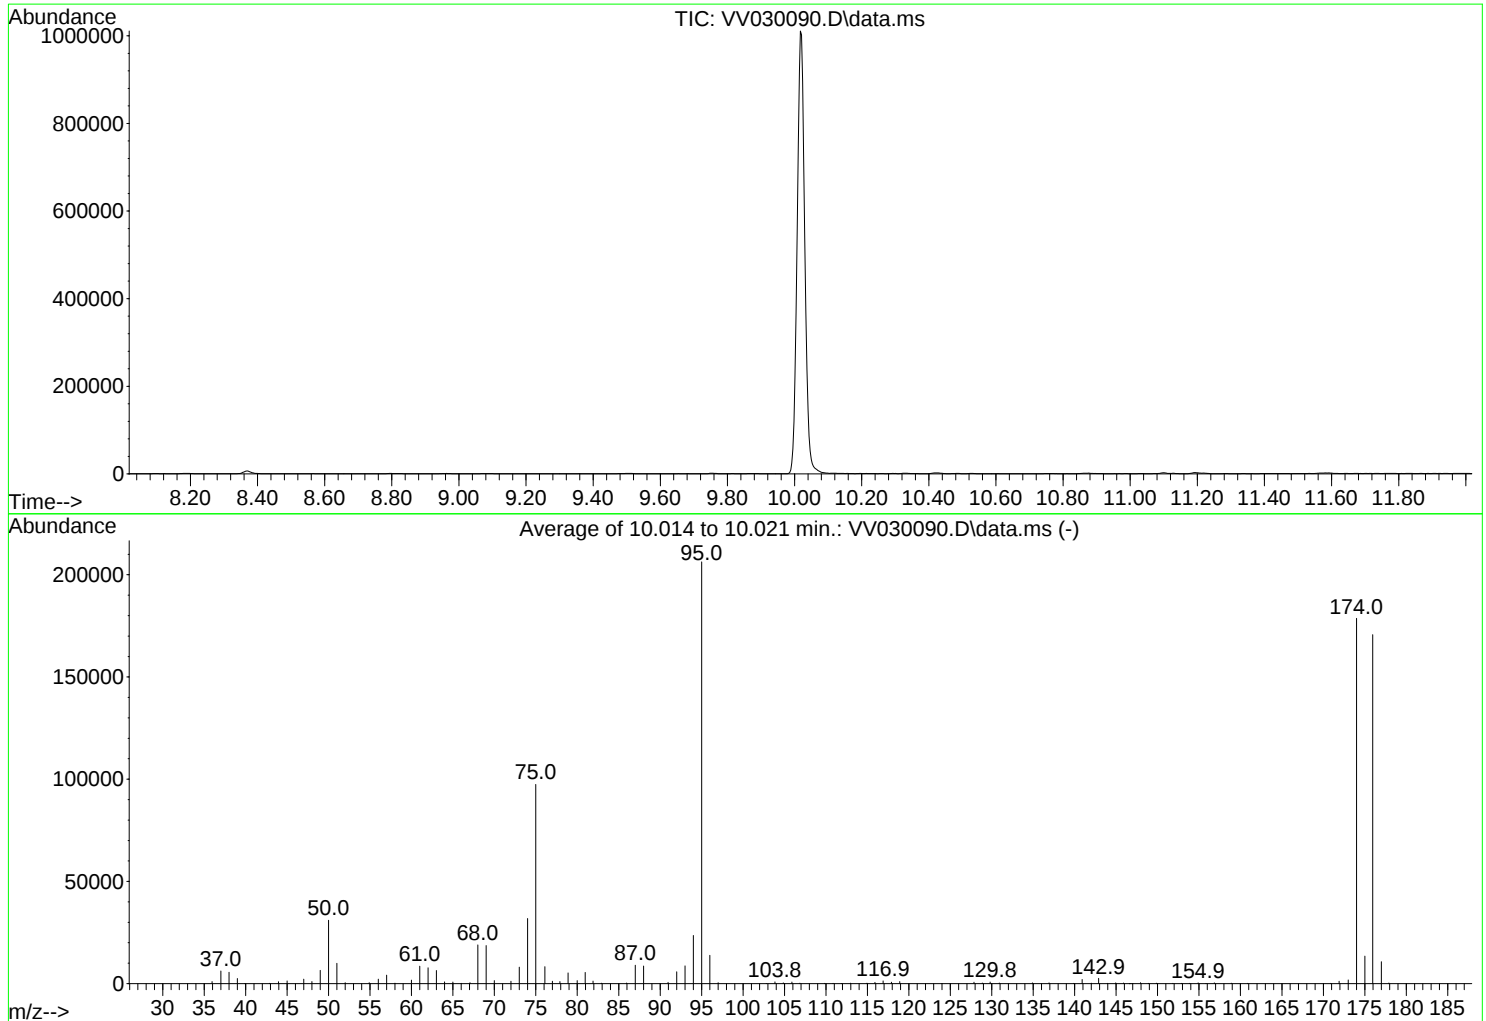

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.0	30960	PASS
75	95	30	80	47.2	97448	PASS
95	95	100	100	100.0	206315	PASS
96	95	5	9	6.7	13823	PASS
173	174	0.00	2	1.0	1769	PASS
174	95	50	120	86.6	178667	PASS
175	174	5	9	7.5	13455	PASS
176	174	95	105	95.5	170667	PASS
177	176	5	10	6.3	10693	PASS

m/z	Abundance
39.90	144.0
43.90	204.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224

m/z	Abundance
36.00	1035.0
37.00	5926.0
38.00	5249.0
39.00	2420.0
40.00	216.0
42.90	139.0
44.00	1153.0
45.00	1372.0
47.00	2026.0
48.00	896.0
49.00	6151.0
50.00	29672.0
51.00	9602.0
52.00	406.0
54.90	418.0
56.00	2159.0
57.00	3927.0
58.00	277.0
60.00	1607.0
61.00	8380.0
62.00	7588.0
63.00	6249.0
64.00	828.0
65.00	820.0
66.00	112.0
67.00	496.0
68.00	18152.0
69.00	17896.0
70.00	1442.0
72.00	1226.0
73.00	7654.0
74.00	30336.0
75.00	92608.0
76.10	8027.0
77.00	1167.0
77.90	958.0
78.90	5083.0
80.00	1468.0
80.90	5267.0
81.90	1178.0
82.90	219.0
86.00	247.0
87.00	8645.0
88.00	8303.0
90.90	655.0
92.00	5302.0
93.00	8105.0
94.00	22192.0
95.00	195776.0
96.00	13355.0
97.00	477.0
103.90	836.0
104.80	342.0
105.90	712.0
106.90	262.0
109.80	120.0
110.90	197.0
111.90	131.0
113.00	227.0
115.00	236.0
115.90	626.0
116.90	1257.0
117.90	608.0
118.90	974.0
127.90	689.0
128.80	290.0
129.80	730.0
130.90	313.0
134.90	391.0
136.90	346.0
140.00	164.0
140.90	1912.0
142.00	242.0
142.90	2411.0
143.90	123.0
144.90	398.0
145.90	230.0
148.00	516.0
148.90	175.0
149.80	237.0
151.80	162.0
152.90	168.0
153.90	155.0
155.00	366.0
155.80	112.0
156.90	312.0
158.90	224.0
160.80	174.0
170.90	155.0
171.90	1141.0
173.00	1638.0
174.00	164096.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224

175.00	12750.0
175.90	156416.0
177.00	10192.0
177.90	304.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224

m/z	Abundance
36.00	1047.0
37.00	6408.0
38.00	5827.0
39.00	2589.0
39.90	201.0
42.90	165.0
44.00	1184.0
45.00	1402.0
47.00	2347.0
48.00	1061.0
49.00	6767.0
50.00	32032.0
51.00	10270.0
52.00	477.0
54.90	475.0
56.00	2280.0
57.00	4225.0
58.00	262.0
60.00	1760.0
61.00	8774.0
62.00	7970.0
63.00	6651.0
64.00	876.0
65.00	785.0
66.00	136.0
67.10	517.0
68.00	19672.0
69.00	19328.0
70.00	1534.0
72.00	1227.0
73.00	8273.0
74.00	33032.0
75.00	100912.0
76.10	8663.0
77.00	1142.0
77.90	1002.0
78.90	5478.0
80.00	1543.0
81.00	5601.0
81.90	1297.0
82.90	233.0
85.90	305.0
87.00	9274.0
88.00	8986.0
90.90	682.0
92.00	5949.0
93.00	9050.0
94.00	24360.0
95.00	213248.0
96.00	14300.0
97.00	505.0
102.80	119.0
103.80	932.0
104.80	384.0
105.90	795.0
106.90	236.0
109.80	129.0
110.90	147.0
111.90	109.0
113.00	219.0
115.00	258.0
115.90	677.0
116.90	1366.0
117.90	716.0
118.90	1086.0
124.00	127.0
127.90	698.0
128.90	308.0
129.80	821.0
130.90	363.0
134.90	433.0
136.90	394.0
139.90	141.0
140.90	2087.0
142.00	263.0
142.90	2689.0
144.00	156.0
144.90	406.0
145.90	288.0
146.90	101.0
147.90	509.0
148.90	194.0
149.90	225.0
151.80	154.0
152.90	166.0
153.90	198.0
154.90	418.0
155.80	116.0
156.80	370.0
158.90	279.0
160.90	191.0
170.80	137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224

171.90	1250.0
173.00	1826.0
174.00	184640.0
175.00	14014.0
176.00	176448.0
177.00	10977.0
177.90	324.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224

m/z	Abundance
35.90	1000.0
37.00	6306.0
38.00	5712.0
39.00	2497.0
39.90	192.0
42.90	160.0
44.00	1108.0
45.00	1273.0
47.00	2315.0
48.00	1030.0
49.00	6603.0
50.00	31176.0
51.00	10014.0
52.00	490.0
54.90	469.0
56.00	2271.0
57.00	4203.0
58.00	194.0
60.00	1711.0
61.00	8425.0
62.00	7796.0
63.00	6382.0
64.00	853.0
65.00	702.0
66.00	132.0
67.10	481.0
68.00	19064.0
69.00	18704.0
70.00	1439.0
72.00	1103.0
73.00	8246.0
74.00	32200.0
75.00	98824.0
76.10	8241.0
77.00	1124.0
77.90	1014.0
78.90	5300.0
80.00	1478.0
81.00	5533.0
81.90	1211.0
82.90	209.0
85.90	334.0
87.00	9147.0
88.00	8586.0
91.00	662.0
92.00	6153.0
93.00	8943.0
94.00	24040.0
95.00	209920.0
96.00	13815.0
97.00	432.0
102.80	124.0
103.90	894.0
104.90	363.0
105.90	848.0
106.80	190.0
109.90	111.0
110.70	122.0
111.80	102.0
112.90	208.0
114.90	247.0
115.90	683.0
116.90	1326.0
117.90	748.0
118.90	1100.0
124.00	119.0
127.80	652.0
128.90	328.0
129.80	794.0
130.90	342.0
134.90	423.0
136.90	358.0
139.80	137.0
140.90	2020.0
142.00	241.0
142.90	2560.0
144.00	174.0
145.00	368.0
145.90	341.0
146.60	109.0
147.90	485.0
148.90	185.0
149.90	193.0
151.90	112.0
152.90	150.0
153.90	200.0
154.80	454.0
155.90	102.0
156.80	404.0
158.90	297.0
160.90	229.0
171.00	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224

171.90	1160.0
173.00	1844.0
174.00	187264.0
175.00	13602.0
176.00	179136.0
177.00	10911.0
177.90	289.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224