




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022824\
Data File : VV034464.D
Acq On : 28 Feb 2024 12:15
Operator : SY/MD
Sample : P1566-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JWAC3

Manual IntegrationsAPPROVED

Quant Time: Feb 29 00:36:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Feb 29 00:34:49 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/29/2024
Supervised By :Semsettin Yesilyurt 02/29/2024

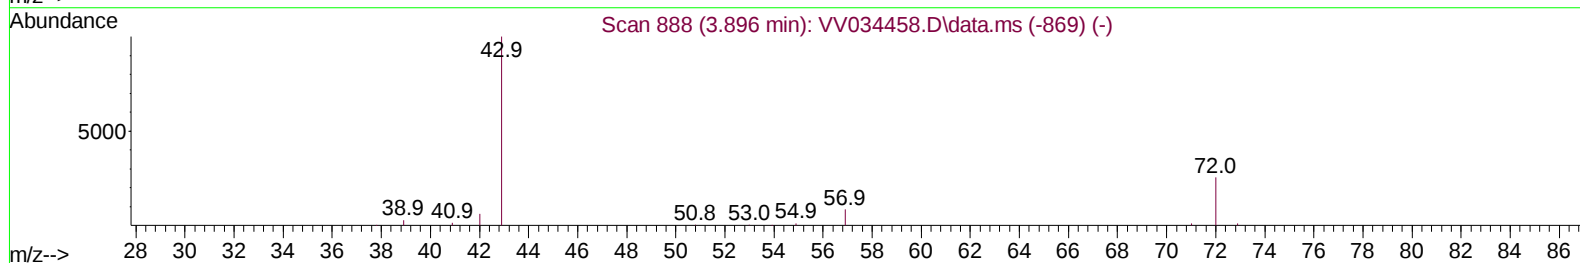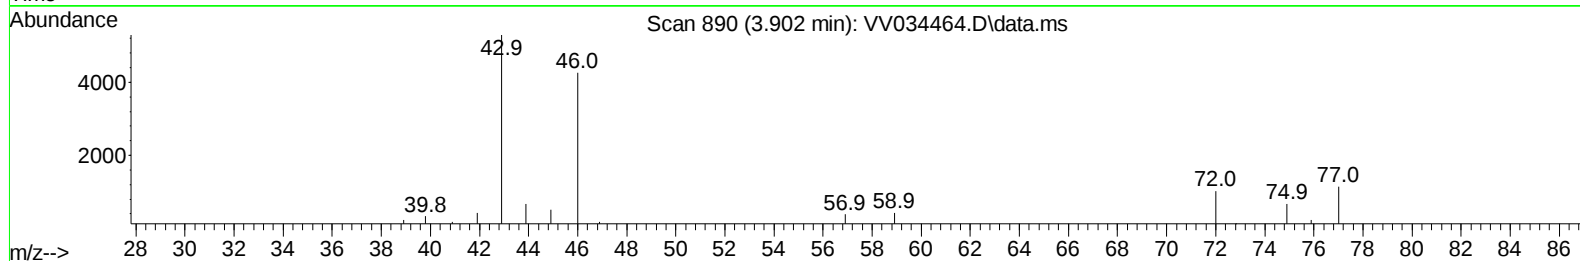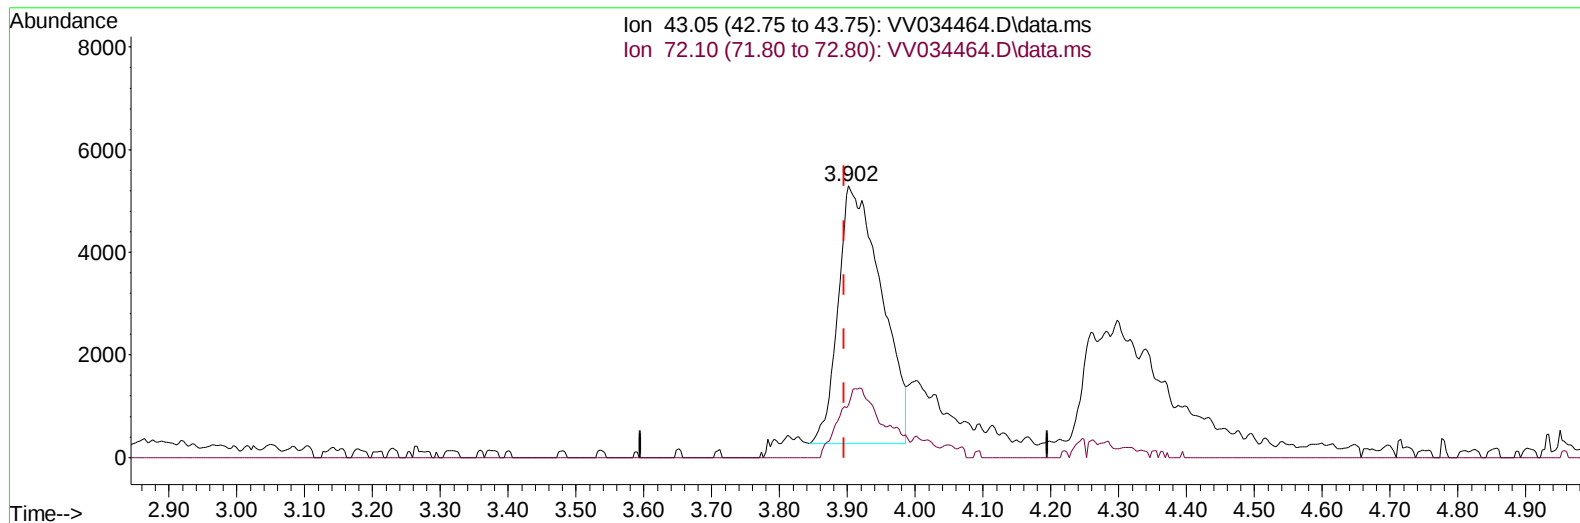

TIC: VV034464.D\data.ms

(21) 2-Butanone (T)

3.902min (+ 0.006) 8.86 ug/L

response 22193

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	24.70	22.32
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022824\
Data File : VV034464.D
Acq On : 28 Feb 2024 12:15
Operator : SY/MD
Sample : P1566-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JWAC3

Manual IntegrationsAPPROVED

Quant Time: Feb 29 00:36:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Feb 29 00:34:49 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/29/2024
Supervised By :Semsettin Yesilyurt 02/29/2024

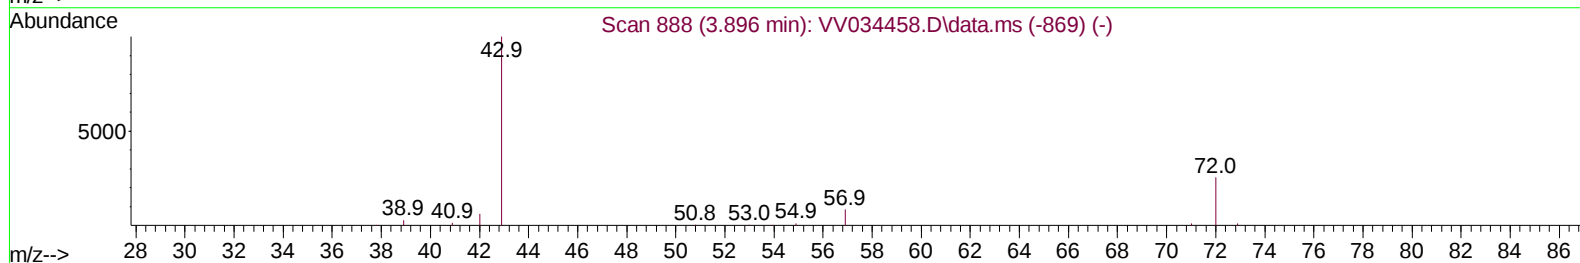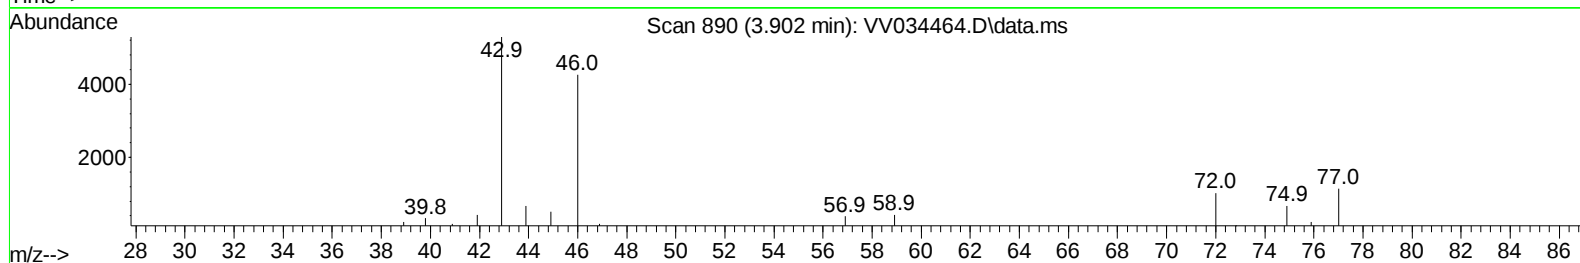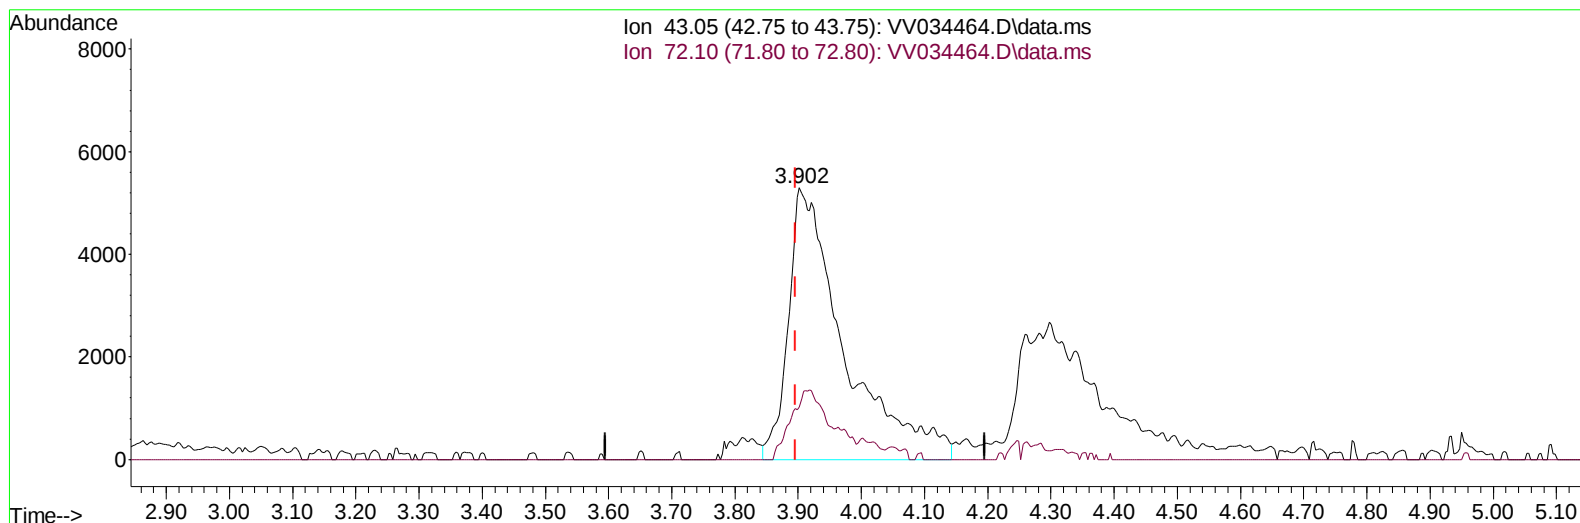

TIC: VV034464.D\data.ms

(21) 2-Butanone (T)

3.902min (+ 0.006) 12.94 ug/L m

response 32415

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	24.70	15.28
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022824\
 Data File : VV034464.D
 Acq On : 28 Feb 2024 12:15
 Operator : SY/MD
 Sample : P1566-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JWAC3

Manual IntegrationsAPPROVED

Quant Time: Feb 29 00:36:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Feb 29 00:34:49 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/29/2024
 Supervised By :Semsettin Yesilyurt 02/29/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.535	114		147818	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117		137105	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152		68873	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		32641	3.804	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.000%	
7) Chloroethane-d5	1.532	69		31019	4.093	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.800%	
11) 1,1-Dichloroethene-d2	2.060	65		15914	3.984	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.600%	
20) 2-Butanone-d5	3.809	46		125363	55.879	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.760%	
24) Chloroform-d	4.249	84		77542	4.501	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.000%	
26) 1,2-Dichloroethane-d4	4.947	65		42889	4.892	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.800%	
32) Benzene-d6	4.963	84		139494	4.523	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.400%	
36) 1,2-Dichloropropane-d6	5.992	67		44222	4.802	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.000%	
41) Toluene-d8	7.246	98		119362	4.315	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.400%	
43) trans-1,3-Dichloroprop...	7.561	79		16099	4.692	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.800%	
46) 2-Hexanone-d5	8.027	63		107094	55.205	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	110.420%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84		36647	5.027	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.600%	
66) 1,2-Dichlorobenzene-d4	11.561	152		50260	4.803	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.000%	
Target Compounds							
						Qvalue	
13) Acetone	2.137	43		337160	147.760	ug/L	98
21) 2-Butanone	3.902	43		32415m	12.940	ug/L	
34) Trichloroethene	5.838	95		20307	2.049	ug/L	98
47) Tetrachloroethene	7.905	164		110129	14.167	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022824\
Data File : VV034464.D
Acq On : 28 Feb 2024 12:15
Operator : SY/MD
Sample : P1566-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JWAC3

Manual IntegrationsAPPROVED

Quant Time: Feb 29 00:36:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Feb 29 00:34:49 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/29/2024
Supervised By :Semsettin Yesilyurt 02/29/2024

